

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
 Data File : VV032143.D
 Acq On : 20 Sep 2023 13:36
 Operator : SY/MD
 Sample : 04417-19ME
 Misc : 4.83g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Sep 21 01:39:04 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 21 01:37:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	247078	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	239467	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.191	152	123925	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	65195	42.162	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	84.320%
7) Chloroethane-d5	1.506	69	12219	9.014	ug/L	-0.02
Spiked Amount	50.000	Range	70 - 130	Recovery	=	18.020%#
11) 1,1-Dichloroethene-d2	2.034	65	25877	35.739	ug/L	-0.03
Spiked Amount	50.000	Range	60 - 125	Recovery	=	71.480%
21) 2-Butanone-d5	3.809	46	86237	70.909	ug/L	0.02
Spiked Amount	100.000	Range	40 - 130	Recovery	=	70.910%
24) Chloroform-d	4.249	84	109497	32.397	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	64.800%#
26) 1,2-Dichloroethane-d4	4.944	65	70828	31.578	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	63.160%#
32) Benzene-d6	4.957	84	230627	35.295	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	70.580%
36) 1,2-Dichloropropane-d6	5.992	67	76784	36.508	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	73.020%
41) Toluene-d8	7.246	98	204598	33.982	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	67.960%#
43) trans-1,3-Dichloroprop...	7.558	79	33909	31.106	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	62.220%
47) 2-Hexanone-d5	8.040	63	24397	37.847	ug/L	0.01
Spiked Amount	100.000	Range	45 - 130	Recovery	=	37.850%#
56) 1,1,2,2-Tetrachloroeth...	10.162	84	97597	35.910	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	71.820%
66) 1,2-Dichlorobenzene-d4	11.567	152	82332	36.445	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	72.880%#
Target Compounds						
61) 1,2,3-Trichloropropane	11.191	75	15898	6.790	ug/L	Qvalue # 67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
Data File : VV032143.D
Acq On : 20 Sep 2023 13:36
Operator : SY/MD
Sample : 04417-19ME
Misc : 4.83g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Sep 21 01:39:04 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 21 01:37:00 2023
Response via : Initial Calibration

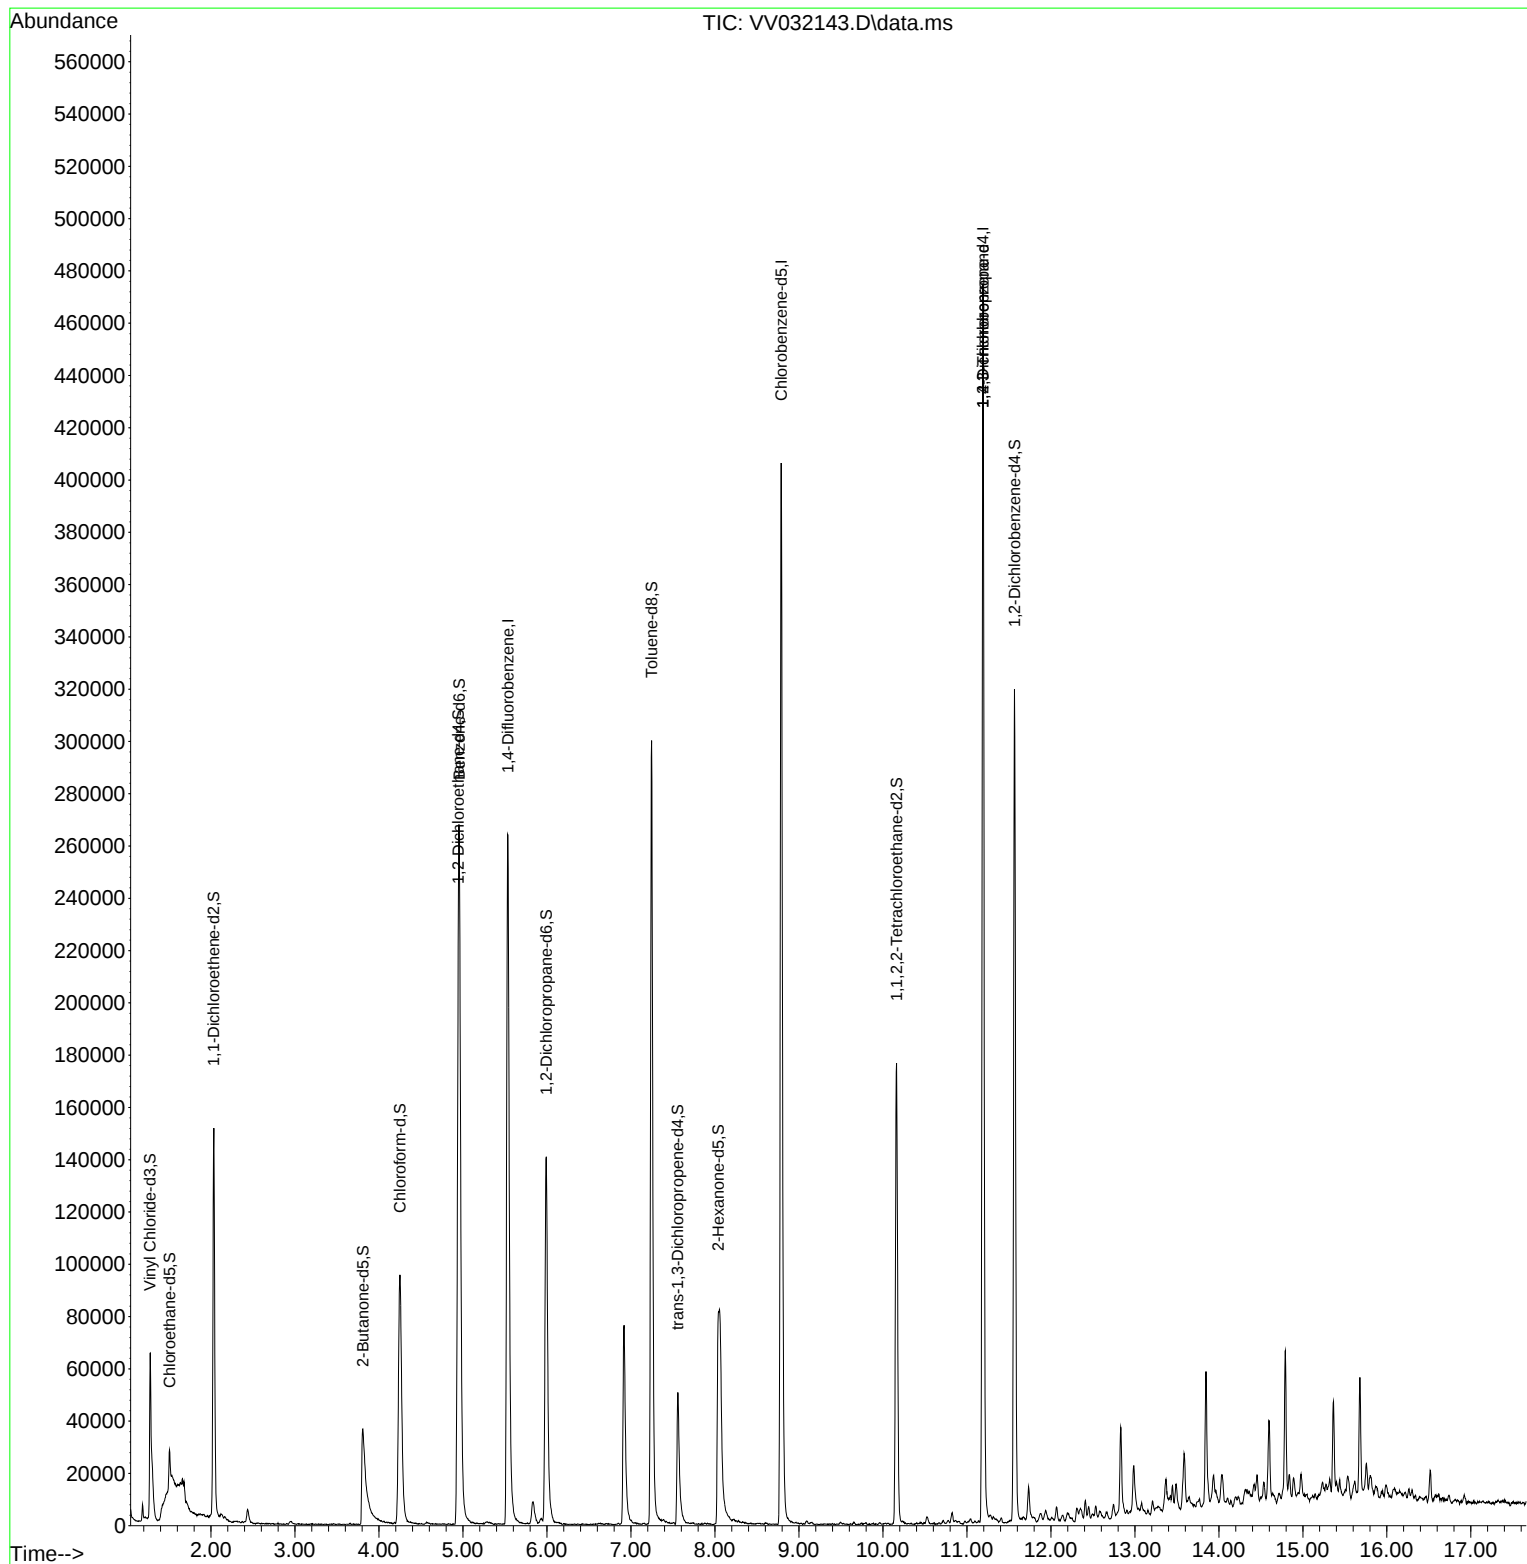

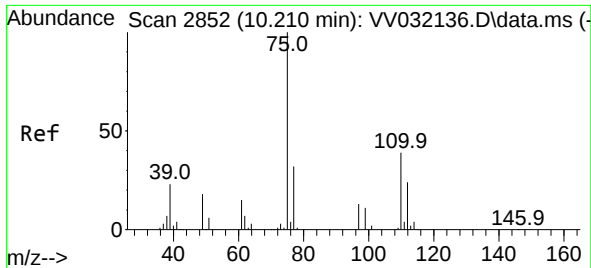

#61
1,2,3-Trichloropropane
Concen: 6.790 ug/L
RT: 11.191 min Scan# 31
Delta R.T. 0.981 min
Lab File: VV032143.D
Acq: 20 Sep 2023 13:36

Instrument :
MSVOA_V
ClientSampleId :

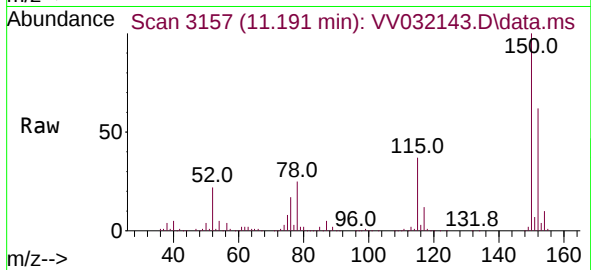

Tgt Ion:	75	Resp:	15898
Ion	Ratio	Lower	Upper
75	100		
77	33.5	25.7	38.5
110	2.0	30.3	45.5#

