

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
 Data File : VV032140.D
 Acq On : 20 Sep 2023 12:26
 Operator : SY/MD
 Sample : 04385-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYP5

Quant Time: Sep 21 01:38:25 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 21 01:37:00 2023
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		5.539	114	212555	50.000	ug/L	0.00
28) Chlorobenzene-d5		8.786	117	204507	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		11.188	152	101625	50.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		1.278	65	85108	63.979	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	127.960%	
7) Chloroethane-d5		1.532	69	70058	60.078	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	120.160%	
11) 1,1-Dichloroethene-d2		2.060	65	34967	56.137	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	112.280%	
21) 2-Butanone-d5		3.786	46	118803	113.553	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	113.550%	
24) Chloroform-d		4.252	84	147398	50.695	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	101.380%	
26) 1,2-Dichloroethane-d4		4.944	65	94018	48.725	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.460%	
32) Benzene-d6		4.963	84	310866	55.707	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	111.420%	
36) 1,2-Dichloropropane-d6		5.992	67	102177	56.887	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	113.780%	
41) Toluene-d8		7.246	98	279566	54.371	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	108.740%	
43) trans-1,3-Dichloroprop...		7.558	79	45994	49.405	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	98.820%	
47) 2-Hexanone-d5		8.027	63	75031	136.293	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	136.290%#	
56) 1,1,2,2-Tetrachloroeth...		10.156	84	128748	55.470	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	110.940%	
66) 1,2-Dichlorobenzene-d4		11.564	152	104882	56.614	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	113.220%	
Target Compounds							Qvalue
13) Acetone		2.114	43	10305	11.066	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
Data File : VV032140.D
Acq On : 20 Sep 2023 12:26
Operator : SY/MD
Sample : 04385-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYP5

Quant Time: Sep 21 01:38:25 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 21 01:37:00 2023
Response via : Initial Calibration

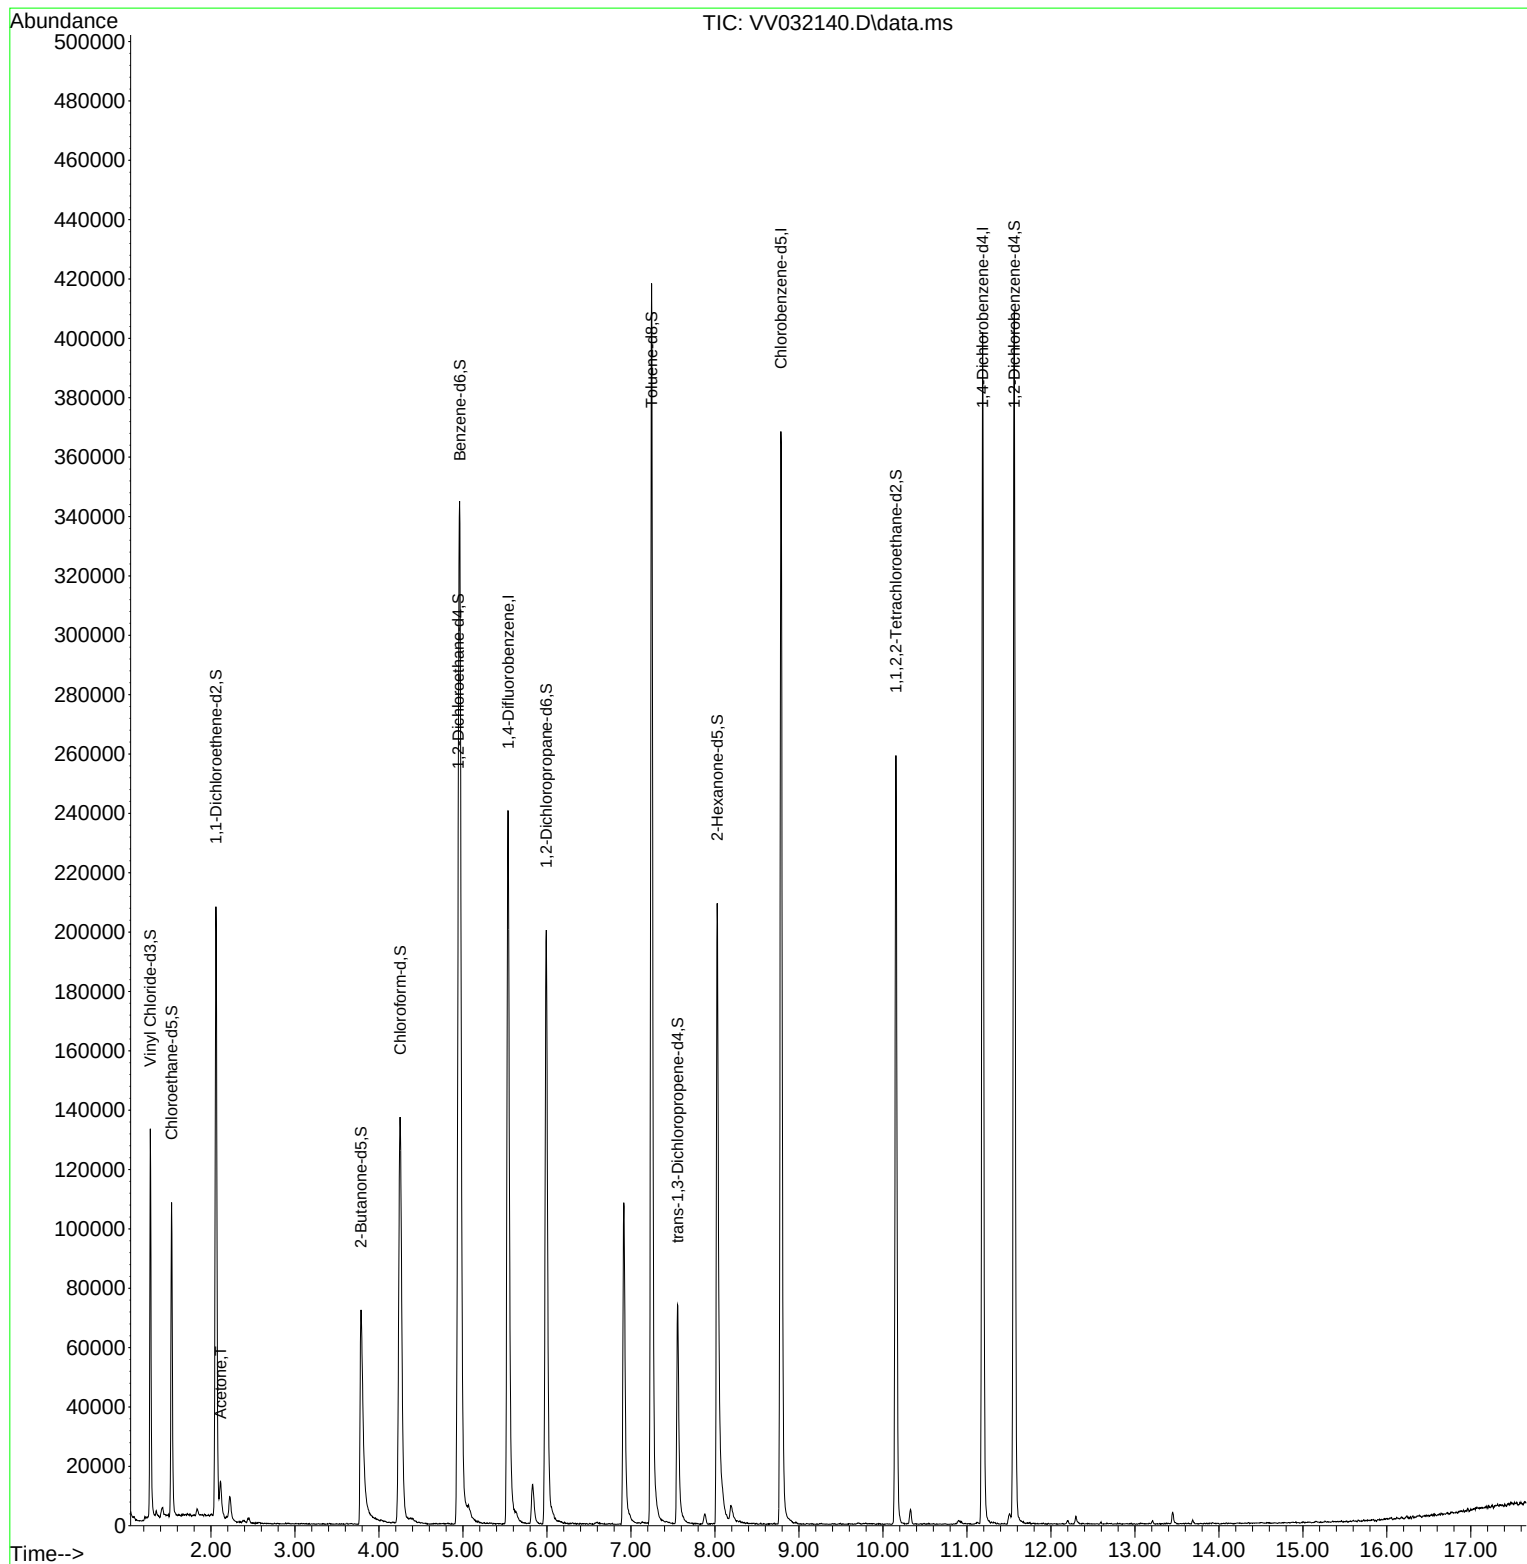

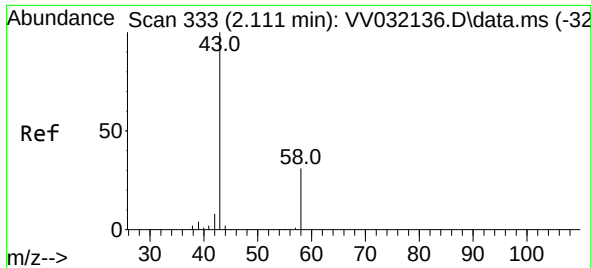

#13

Acetone

Concen: 11.066 ug/L

RT: 2.114 min Scan# 31

Delta R.T. 0.003 min

Lab File: VV032140.D

Acq: 20 Sep 2023 12:26

Instrument :

MSVOA_V

ClientSampleId :

EZYP5

Tgt Ion: 43 Resp: 10305

Ion Ratio Lower Upper

43 100

58 31.1 0.0 61.0

