

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
 Data File : VV032137.D
 Acq On : 20 Sep 2023 11:13
 Operator : SY/MD
 Sample : VV0920MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK396

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV032137.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	117639	123385	15.39%	1.887%
2	1.529	145	152	168	rVB	92535	111823	13.95%	1.710%
3	2.059	308	317	333	rBV	177366	257132	32.08%	3.933%
4	2.445	431	437	438	rBV4	1604	1549	0.19%	0.024%
5	2.641	496	498	499	rBV	245	98	0.01%	0.001%
6	2.703	510	517	526	rVB5	1499	2012	0.25%	0.031%
7	2.950	590	594	598	rBV2	326	270	0.03%	0.004%
8	3.002	606	610	613	rBV2	335	251	0.03%	0.004%
9	3.108	640	643	646	rBV3	332	245	0.03%	0.004%
10	3.169	659	662	664	rVB	218	120	0.01%	0.002%
11	3.256	685	689	692	rBV	182	155	0.02%	0.002%
12	3.272	692	694	702	rVB	271	203	0.03%	0.003%
13	3.426	740	742	746	rBV2	222	142	0.02%	0.002%
14	3.519	767	771	773	rBV	339	153	0.02%	0.002%
15	3.535	773	776	781	rVV2	406	255	0.03%	0.004%
16	3.564	782	785	789	rVB2	325	231	0.03%	0.004%
17	3.584	789	791	793	rBV	255	129	0.02%	0.002%
18	3.686	819	823	826	rVB3	249	195	0.02%	0.003%
19	3.722	832	834	837	rVB3	212	98	0.01%	0.001%
20	3.786	845	854	894	rBV	58005	161487	20.15%	2.470%
21	4.249	981	998	1031	rBV	119165	314191	39.20%	4.806%
22	4.558	1090	1094	1097	rBV4	298	319	0.04%	0.005%
23	4.657	1121	1125	1127	rBV3	229	166	0.02%	0.003%
24	4.715	1141	1143	1145	rBV	279	109	0.01%	0.002%
25	4.799	1167	1169	1172	rBV2	271	186	0.02%	0.003%
26	4.844	1180	1183	1187	rBV3	334	295	0.04%	0.005%
27	4.956	1201	1218	1242	rBV2	306693	801544	100.00%	12.261%
28	5.378	1347	1349	1351	rVB	336	177	0.02%	0.003%
29	5.407	1356	1358	1365	rVB3	301	332	0.04%	0.005%
30	5.535	1386	1398	1427	rBV	273743	570657	71.19%	8.729%
31	5.828	1479	1489	1508	rBV3	9458	20395	2.54%	0.312%
32	5.989	1525	1539	1572	rBV	174253	372764	46.51%	5.702%
33	6.204	1604	1606	1608	rBV	271	98	0.01%	0.001%
34	6.310	1637	1639	1643	rVB2	201	97	0.01%	0.001%
35	6.381	1658	1661	1663	rBV	172	123	0.02%	0.002%
36	6.435	1675	1678	1681	rBV3	331	179	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
 Data File : VV032137.D
 Acq On : 20 Sep 2023 11:13
 Operator : SY/MD
 Sample : VV0920MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK396

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	6.667	1748	1750	1752	rVB	245	112	0.01%	0.002%
38	6.680	1752	1754	1757	rVB2	295	153	0.02%	0.002%
39	6.760	1777	1779	1784	rVB2	177	128	0.02%	0.002%
40	6.796	1784	1790	1792	rBV	198	181	0.02%	0.003%
41	6.915	1815	1827	1858	rBV2	95497	187704	23.42%	2.871%
42	7.246	1918	1930	1965	rBV	358315	655809	81.82%	10.031%
43	7.554	2016	2026	2048	rBV	65675	122455	15.28%	1.873%
44	7.789	2096	2099	2104	rVB2	446	337	0.04%	0.005%
45	7.812	2104	2106	2109	rVB	260	166	0.02%	0.003%
46	7.828	2109	2111	2114	rVB	211	98	0.01%	0.001%
47	7.847	2114	2117	2120	rBV2	345	178	0.02%	0.003%
48	7.870	2120	2124	2128	rBV3	406	316	0.04%	0.005%
49	7.915	2132	2138	2146	rVB5	788	832	0.10%	0.013%
50	7.956	2148	2151	2157	rVB3	240	210	0.03%	0.003%
51	8.027	2164	2173	2212	rBV	174813	346504	43.23%	5.300%
52	8.516	2323	2325	2328	rVB	439	206	0.03%	0.003%
53	8.567	2339	2341	2345	rVB2	263	170	0.02%	0.003%
54	8.590	2345	2348	2350	rBV	214	177	0.02%	0.003%
55	8.625	2357	2359	2361	rVB2	381	131	0.02%	0.002%
56	8.738	2392	2394	2397	rVB	315	167	0.02%	0.003%
57	8.786	2397	2409	2439	rBV	421231	706333	88.12%	10.804%
58	9.043	2486	2489	2490	rBV	290	123	0.02%	0.002%
59	9.082	2495	2501	2514	rVB5	1212	2036	0.25%	0.031%
60	9.133	2514	2517	2519	rBV	233	119	0.01%	0.002%
61	9.204	2538	2539	2543	rVV	314	179	0.02%	0.003%
62	9.329	2576	2578	2580	rBV	359	92	0.01%	0.001%
63	9.448	2613	2615	2619	rVB2	255	139	0.02%	0.002%
64	9.487	2620	2627	2631	rBV6	1722	2101	0.26%	0.032%
65	9.554	2646	2648	2653	rVB2	321	183	0.02%	0.003%
66	9.615	2662	2667	2670	rBV	119	123	0.02%	0.002%
67	9.693	2688	2691	2694	rBV	221	117	0.01%	0.002%
68	9.767	2710	2714	2716	rBV2	219	131	0.02%	0.002%
69	9.879	2740	2749	2757	rBV6	2204	3325	0.41%	0.051%
70	9.918	2757	2761	2764	rVV2	221	137	0.02%	0.002%
71	10.088	2811	2814	2815	rBV	160	99	0.01%	0.002%
72	10.101	2815	2818	2820	rVB2	251	92	0.01%	0.001%
73	10.156	2823	2835	2862	rBV	228666	365535	45.60%	5.591%
74	10.316	2883	2885	2888	rBV2	179	101	0.01%	0.002%
75	10.487	2928	2938	2944	rBV3	1737	2279	0.28%	0.035%
76	10.522	2947	2949	2951	rBV2	216	98	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
 Data File : VV032137.D
 Acq On : 20 Sep 2023 11:13
 Operator : SY/MD
 Sample : VV0920MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK396

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	10.590	2966	2970	2971	rBV	190	121	0.02%	0.002%
78	10.705	3004	3006	3010	rBB2	179	107	0.01%	0.002%
79	10.863	3047	3055	3063	rBV3	2457	3389	0.42%	0.052%
80	10.966	3084	3087	3089	rVV3	179	98	0.01%	0.001%
81	11.127	3131	3137	3145	rVB5	3113	4349	0.54%	0.067%
82	11.188	3145	3156	3182	rBV	455735	702499	87.64%	10.746%
83	11.365	3207	3211	3214	rBV4	452	366	0.05%	0.006%
84	11.422	3227	3229	3233	rBV	189	113	0.01%	0.002%
85	11.564	3261	3273	3297	rBV	368644	577680	72.07%	8.836%
86	11.818	3349	3352	3353	rBV	424	227	0.03%	0.003%
87	12.056	3423	3426	3427	rBV	220	114	0.01%	0.002%
88	12.281	3494	3496	3499	rVB2	244	122	0.02%	0.002%
89	12.300	3499	3502	3506	rBV2	194	207	0.03%	0.003%
90	12.368	3520	3523	3525	rBV3	681	463	0.06%	0.007%
91	12.532	3571	3574	3577	rBV	192	141	0.02%	0.002%
92	12.590	3584	3592	3602	rBV4	4715	7434	0.93%	0.114%
93	13.207	3776	3784	3795	rBV2	9301	13727	1.71%	0.210%
94	13.445	3846	3858	3874	rBV	39864	65350	8.15%	1.000%
95	13.593	3901	3904	3907	rBV2	251	173	0.02%	0.003%
96	13.686	3925	3933	3946	rVV2	12719	18876	2.35%	0.289%
97	13.737	3946	3949	3956	rVB2	442	388	0.05%	0.006%
98	13.837	3977	3980	3984	rBV2	271	207	0.03%	0.003%
99	13.953	4012	4016	4021	rBV3	371	363	0.05%	0.006%
100	14.197	4090	4092	4094	rBV3	249	96	0.01%	0.001%




Sum of corrected areas: 6537551

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
Data File : VV032137.D
Acq On : 20 Sep 2023 11:13
Operator : SY/MD
Sample : VV0920MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK396

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

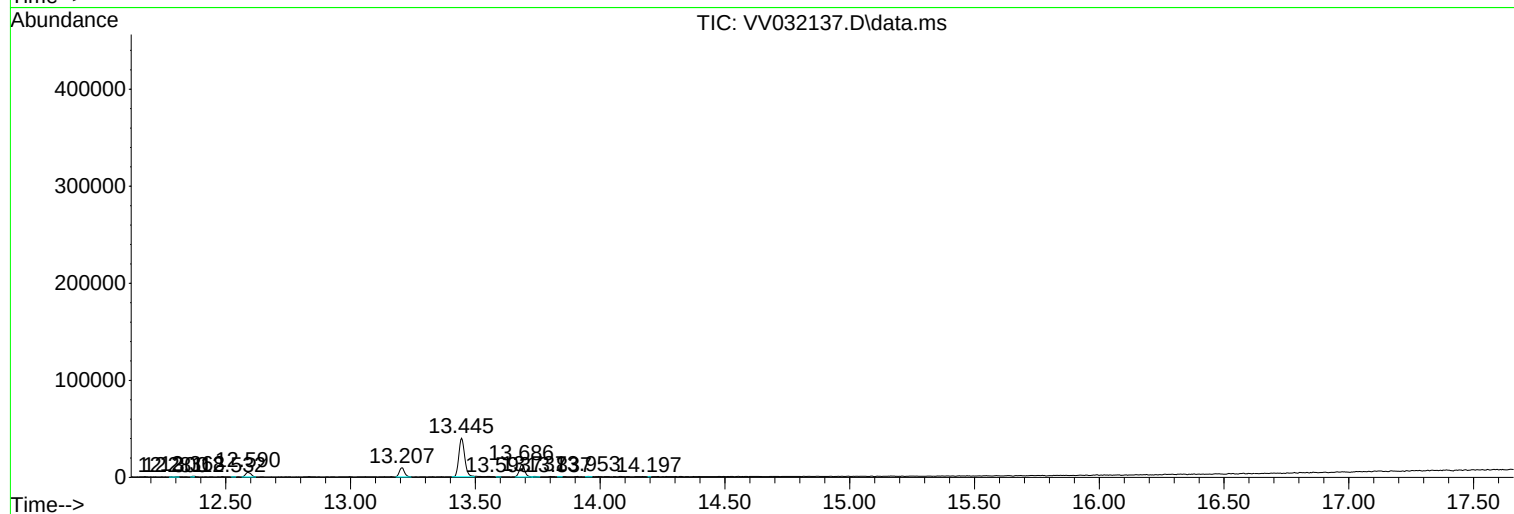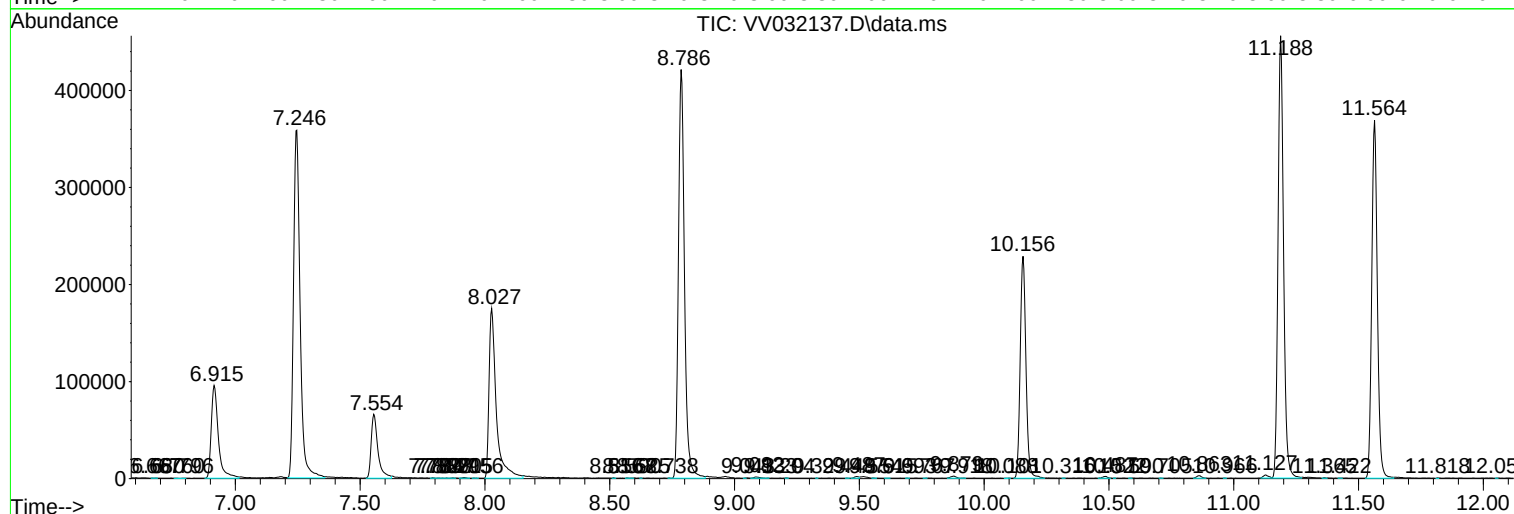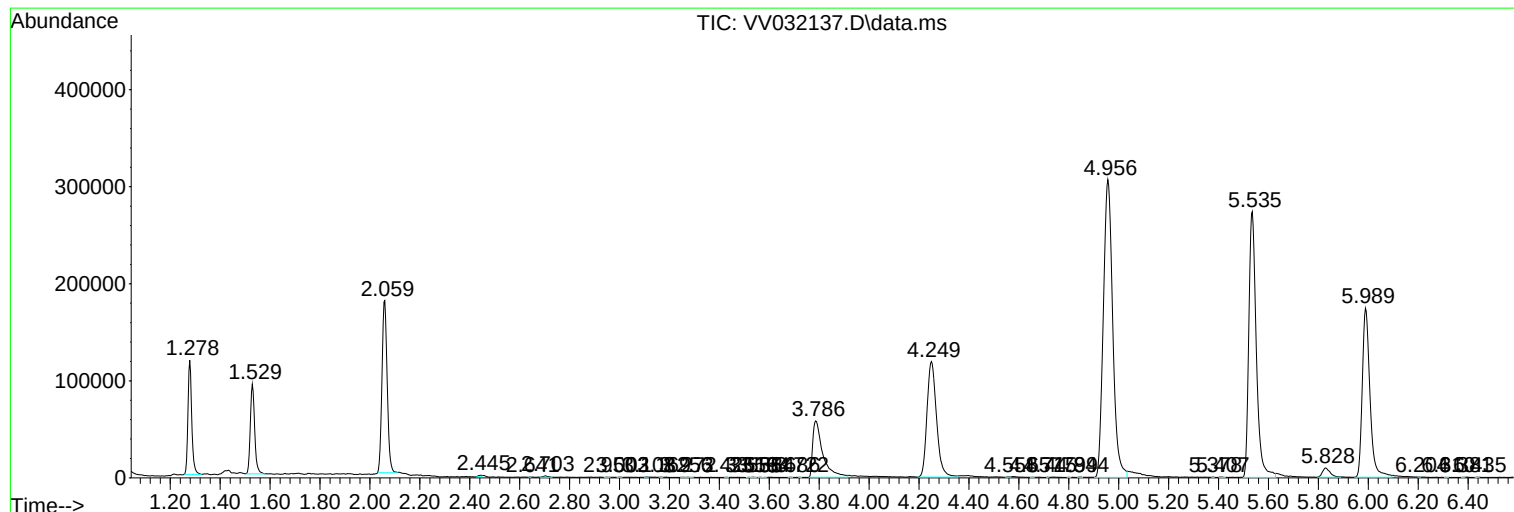

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
Data File : VV032137.D
Acq On : 20 Sep 2023 11:13
Operator : SY/MD
Sample : VV0920MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK396

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
Data File : VV032137.D
Acq On : 20 Sep 2023 11:13
Operator : SY/MD
Sample : VV0920MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK396

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------