

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
 Data File : VV032139.D
 Acq On : 20 Sep 2023 12:03
 Operator : SY/MD
 Sample : 04440-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV032139.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	92	rVB	104734	109731	14.62%	1.820%
2	1.532	146	153	168	rVB	84063	99524	13.26%	1.651%
3	2.060	308	317	332	rBV	163514	236865	31.55%	3.929%
4	2.452	431	439	454	rVB7	2151	3900	0.52%	0.065%
5	2.577	475	478	480	rBV2	227	116	0.02%	0.002%
6	2.635	493	496	498	rBV	355	174	0.02%	0.003%
7	2.754	530	533	539	rVB3	315	248	0.03%	0.004%
8	2.802	546	548	551	rBV	221	164	0.02%	0.003%
9	2.902	576	579	584	rBV2	179	110	0.01%	0.002%
10	3.124	642	648	652	rBV2	296	368	0.05%	0.006%
11	3.166	658	661	664	rBV	142	105	0.01%	0.002%
12	3.220	676	678	680	rVB2	240	86	0.01%	0.001%
13	3.240	681	684	686	rBV2	243	159	0.02%	0.003%
14	3.355	717	720	722	rVB2	294	125	0.02%	0.002%
15	3.371	722	725	726	rBV2	170	104	0.01%	0.002%
16	3.394	731	732	736	rVB	211	97	0.01%	0.002%
17	3.420	736	740	741	rBV	327	188	0.03%	0.003%
18	3.561	779	784	786	rBV	126	117	0.02%	0.002%
19	3.584	789	791	794	rVB	257	98	0.01%	0.002%
20	3.667	815	817	820	rVB2	192	91	0.01%	0.002%
21	3.725	830	835	838	rBV2	286	239	0.03%	0.004%
22	3.789	846	855	895	rBV	58470	161845	21.56%	2.685%
23	4.252	983	999	1022	rBV	111090	289692	38.59%	4.806%
24	4.632	1114	1117	1118	rBV	204	114	0.02%	0.002%
25	4.728	1145	1147	1153	rVB2	284	247	0.03%	0.004%
26	4.815	1170	1174	1175	rBV	170	84	0.01%	0.001%
27	4.860	1184	1188	1190	rBV2	219	180	0.02%	0.003%
28	4.876	1190	1193	1194	rBV	185	83	0.01%	0.001%
29	4.960	1202	1219	1244	rBV2	283611	750708	100.00%	12.453%
30	5.387	1349	1352	1353	rBV2	209	116	0.02%	0.002%
31	5.539	1387	1399	1429	rBV	251769	528388	70.39%	8.765%
32	5.828	1479	1489	1509	rBV3	9842	21555	2.87%	0.358%
33	5.944	1522	1525	1526	rBV2	280	152	0.02%	0.003%
34	5.992	1527	1540	1576	rVV	164974	352322	46.93%	5.845%
35	6.246	1617	1619	1625	rVB3	401	253	0.03%	0.004%
36	6.342	1646	1649	1652	rBV2	164	124	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
 Data File : VV032139.D
 Acq On : 20 Sep 2023 12:03
 Operator : SY/MD
 Sample : 04440-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	6.452	1678	1683	1687	rBV	224	220	0.03%	0.004%
38	6.574	1719	1721	1724	rBV2	473	206	0.03%	0.003%
39	6.600	1724	1729	1732	rBV4	433	408	0.05%	0.007%
40	6.764	1778	1780	1783	rVB2	197	84	0.01%	0.001%
41	6.918	1816	1828	1854	rBV	88882	174802	23.28%	2.900%
42	7.140	1891	1897	1900	rBV5	639	766	0.10%	0.013%
43	7.246	1917	1930	1969	rBV	334254	603481	80.39%	10.011%
44	7.558	2017	2027	2050	rBV	60443	113752	15.15%	1.887%
45	7.796	2097	2101	2102	rBV	420	207	0.03%	0.003%
46	7.854	2117	2119	2121	rVB	230	115	0.02%	0.002%
47	7.873	2121	2125	2129	rBV2	231	260	0.03%	0.004%
48	7.915	2135	2138	2141	rVB2	411	293	0.04%	0.005%
49	7.928	2141	2142	2147	rVB	171	93	0.01%	0.002%
50	7.960	2147	2152	2153	rBV	138	104	0.01%	0.002%
51	8.027	2164	2173	2216	rBV	168180	345505	46.02%	5.732%
52	8.503	2319	2321	2326	rVB3	333	165	0.02%	0.003%
53	8.548	2332	2335	2340	rVB2	216	163	0.02%	0.003%
54	8.606	2350	2353	2356	rBV	241	213	0.03%	0.004%
55	8.747	2393	2397	2398	rBV	236	120	0.02%	0.002%
56	8.786	2398	2409	2440	rBV	389917	658769	87.75%	10.928%
57	8.953	2459	2461	2462	rBV	576	205	0.03%	0.003%
58	9.040	2486	2488	2490	rVB	202	87	0.01%	0.001%
59	9.082	2498	2501	2503	rBV	418	306	0.04%	0.005%
60	9.108	2508	2509	2513	rVB3	423	200	0.03%	0.003%
61	9.458	2615	2618	2622	rBV2	117	95	0.01%	0.002%
62	9.484	2622	2626	2627	rBV	510	331	0.04%	0.005%
63	9.526	2637	2639	2646	rVB3	524	433	0.06%	0.007%
64	9.644	2673	2676	2679	rBV	189	133	0.02%	0.002%
65	9.873	2742	2747	2751	rBV3	622	727	0.10%	0.012%
66	10.072	2806	2809	2811	rBV	128	92	0.01%	0.002%
67	10.111	2819	2821	2823	rBV	283	147	0.02%	0.002%
68	10.156	2823	2835	2853	rBV	221470	352994	47.02%	5.856%
69	10.294	2874	2878	2882	rBV2	252	185	0.02%	0.003%
70	10.320	2884	2886	2887	rBV2	208	100	0.01%	0.002%
71	10.439	2919	2923	2925	rBV2	149	124	0.02%	0.002%
72	10.477	2931	2935	2936	rBV2	652	352	0.05%	0.006%
73	10.603	2972	2974	2979	rVB	149	91	0.01%	0.002%
74	10.738	3014	3016	3019	rBV2	181	104	0.01%	0.002%
75	10.873	3048	3058	3065	rVB4	586	1054	0.14%	0.017%
76	10.963	3083	3086	3088	rBV	264	175	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
 Data File : VV032139.D
 Acq On : 20 Sep 2023 12:03
 Operator : SY/MD
 Sample : 04440-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	11.069	3117	3119	3121	rBV	194	92	0.01%	0.002%
78	11.101	3126	3129	3130	rBV	185	92	0.01%	0.002%
79	11.133	3133	3139	3144	rVB3	1095	1096	0.15%	0.018%
80	11.188	3144	3156	3180	rBV	422867	651077	86.73%	10.801%
81	11.381	3213	3216	3219	rBV2	270	233	0.03%	0.004%
82	11.564	3260	3273	3293	rBV	344538	541423	72.12%	8.982%
83	11.731	3323	3325	3328	rVB2	462	261	0.03%	0.004%
84	11.914	3379	3382	3385	rBV2	184	122	0.02%	0.002%
85	12.140	3449	3452	3454	rBV	179	108	0.01%	0.002%
86	12.410	3531	3536	3539	rBV2	259	268	0.04%	0.004%
87	12.590	3587	3592	3601	rVB4	1119	1149	0.15%	0.019%
88	12.840	3666	3670	3672	rBV	185	129	0.02%	0.002%
89	12.937	3699	3700	3704	rBV2	171	112	0.01%	0.002%
90	13.159	3767	3769	3773	rBV2	191	123	0.02%	0.002%
91	13.207	3778	3784	3794	rVV5	1652	2489	0.33%	0.041%
92	13.291	3807	3810	3812	rBV2	259	181	0.02%	0.003%
93	13.332	3821	3823	3826	rBV	216	163	0.02%	0.003%
94	13.368	3832	3834	3836	rBV	199	112	0.01%	0.002%
95	13.448	3851	3859	3871	rBV2	6061	9759	1.30%	0.162%
96	13.631	3913	3916	3919	rBV2	223	144	0.02%	0.002%
97	13.689	3928	3934	3943	rVB6	1847	2487	0.33%	0.041%
98	13.757	3953	3955	3958	rBV2	219	89	0.01%	0.001%
99	13.930	4006	4009	4011	rBV2	244	178	0.02%	0.003%
100	14.390	4150	4152	4156	rVB2	309	144	0.02%	0.002%




Sum of corrected areas: 6028164

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
Data File : VV032139.D
Acq On : 20 Sep 2023 12:03
Operator : SY/MD
Sample : 04440-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

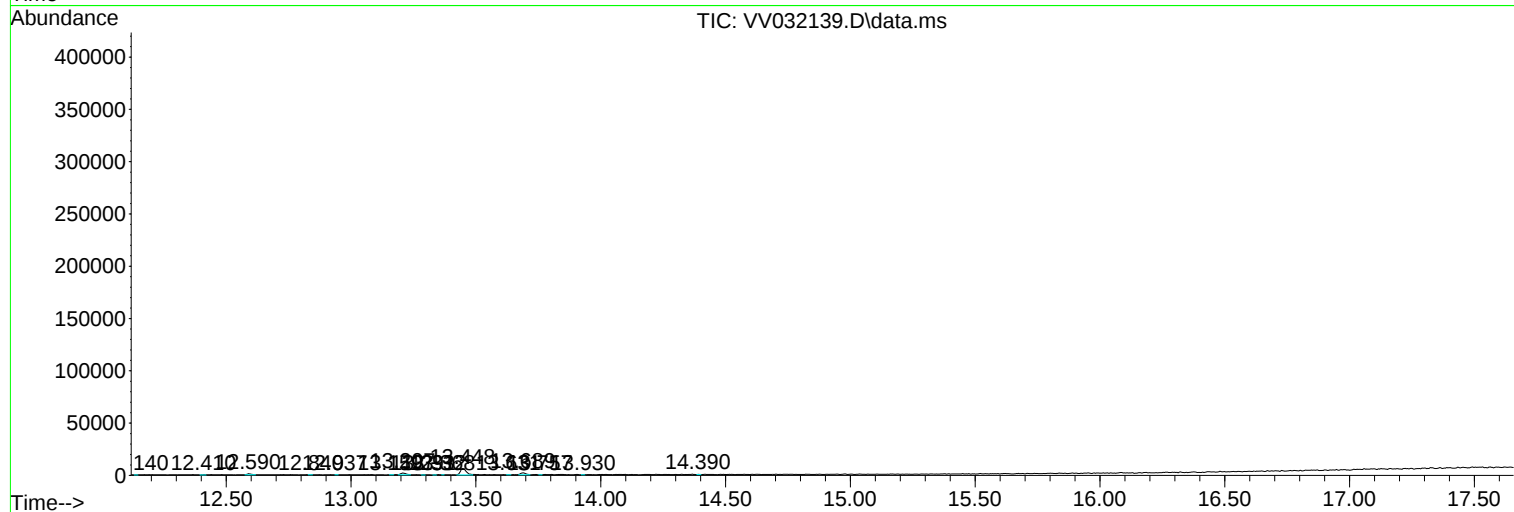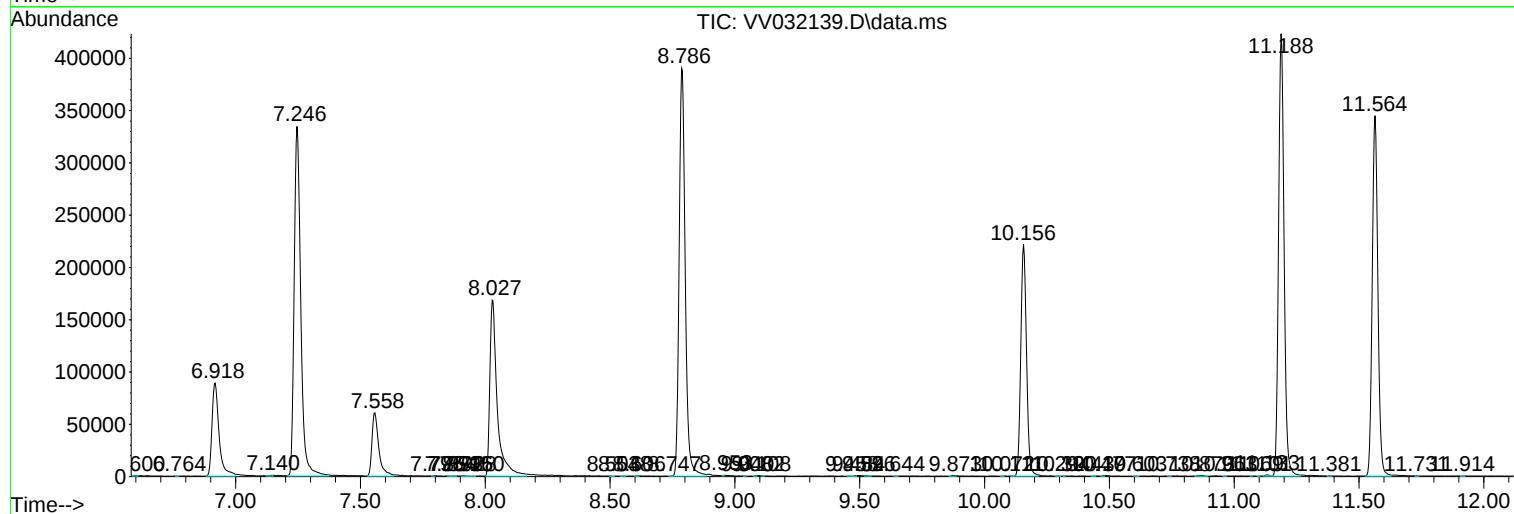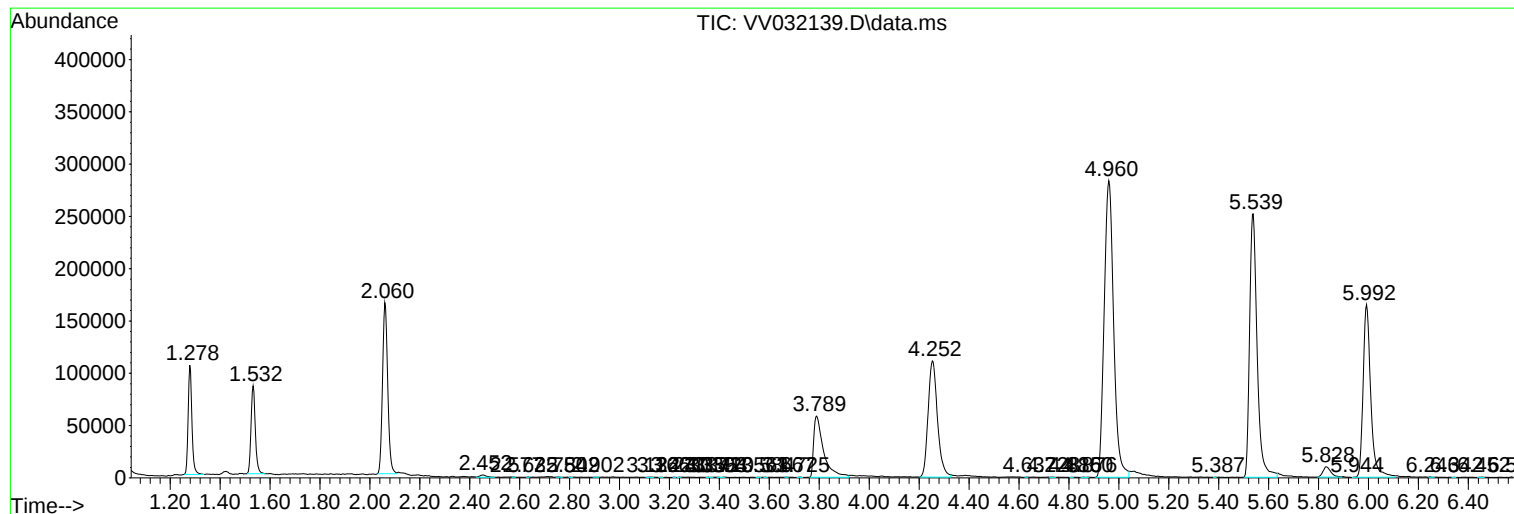

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
Data File : VV032139.D
Acq On : 20 Sep 2023 12:03
Operator : SY/MD
Sample : 04440-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
Data File : VV032139.D
Acq On : 20 Sep 2023 12:03
Operator : SY/MD
Sample : 04440-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc