

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
 Data File : VV032140.D
 Acq On : 20 Sep 2023 12:26
 Operator : SY/MD
 Sample : 04385-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYP5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV032140.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	89	rBV	130620	137738	15.09%	2.023%
2	1.532	146	153	170	rVB	105326	125833	13.79%	1.848%
3	2.060	308	317	328	rBV	203883	293854	32.20%	4.315%
4	2.503	453	455	459	rVB2	358	214	0.02%	0.003%
5	2.526	460	462	464	rVB	416	146	0.02%	0.002%
6	2.725	522	524	528	rVB2	216	109	0.01%	0.002%
7	2.757	532	534	537	rVV	274	192	0.02%	0.003%
8	2.786	541	543	548	rVV	218	179	0.02%	0.003%
9	2.889	573	575	577	rVB2	378	170	0.02%	0.002%
10	2.905	577	580	582	rBV	205	140	0.02%	0.002%
11	3.063	624	629	631	rBV2	225	177	0.02%	0.003%
12	3.201	666	672	675	rBV	168	190	0.02%	0.003%
13	3.555	778	782	784	rBV	200	113	0.01%	0.002%
14	3.619	800	802	807	rVB	281	138	0.02%	0.002%
15	3.645	807	810	812	rBV2	161	114	0.01%	0.002%
16	3.709	826	830	836	rVB2	178	197	0.02%	0.003%
17	3.786	844	854	888	rBV	72207	196482	21.53%	2.885%
18	4.252	983	999	1024	rBV	136538	352688	38.65%	5.179%
19	4.622	1111	1114	1117	rVB2	223	137	0.02%	0.002%
20	4.641	1117	1120	1122	rBV	253	188	0.02%	0.003%
21	4.661	1124	1126	1129	rVV2	218	129	0.01%	0.002%
22	4.680	1129	1132	1136	rVB2	225	181	0.02%	0.003%
23	4.738	1148	1150	1154	rBV2	179	121	0.01%	0.002%
24	4.796	1165	1168	1169	rBV2	190	133	0.01%	0.002%
25	4.818	1173	1175	1178	rVV2	236	162	0.02%	0.002%
26	4.867	1187	1190	1194	rBV2	347	210	0.02%	0.003%
27	4.902	1198	1201	1202	rBV	266	141	0.02%	0.002%
28	4.960	1202	1219	1247	rBV2	344488	912599	100.00%	13.401%
29	5.368	1343	1346	1348	rBV2	265	178	0.02%	0.003%
30	5.481	1379	1381	1384	rBV2	209	128	0.01%	0.002%
31	5.535	1387	1398	1421	rBV	240097	496102	54.36%	7.285%
32	5.831	1479	1490	1516	rVB2	13229	29749	3.26%	0.437%
33	5.992	1524	1540	1558	rBV	200180	416508	45.64%	6.116%
34	6.207	1606	1607	1612	rVB2	530	353	0.04%	0.005%
35	6.275	1625	1628	1631	rBV	352	253	0.03%	0.004%
36	6.362	1653	1655	1658	rBV	294	176	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
 Data File : VV032140.D
 Acq On : 20 Sep 2023 12:26
 Operator : SY/MD
 Sample : 04385-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYP5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	6.426	1672	1675	1678	rBV	223	178	0.02%	0.003%
38	6.474	1686	1690	1694	rVB2	299	265	0.03%	0.004%
39	6.510	1694	1701	1704	rBV	328	326	0.04%	0.005%
40	6.571	1717	1720	1721	rBV	356	173	0.02%	0.003%
41	6.915	1817	1827	1857	rBV	108375	210954	23.12%	3.098%
42	7.246	1918	1930	1968	rBV	417855	745131	81.65%	10.942%
43	7.555	2015	2026	2057	rBV	73768	136803	14.99%	2.009%
44	7.751	2084	2087	2088	rBV	330	170	0.02%	0.002%
45	7.773	2092	2094	2096	rBV	277	124	0.01%	0.002%
46	7.879	2116	2127	2140	rVB2	3539	6557	0.72%	0.096%
47	7.960	2146	2152	2155	rBV2	229	238	0.03%	0.003%
48	7.985	2157	2160	2163	rBV	214	133	0.01%	0.002%
49	8.027	2163	2173	2207	rBV	209078	409155	44.83%	6.008%
50	8.580	2343	2345	2346	rBV	245	120	0.01%	0.002%
51	8.622	2355	2358	2360	rBV2	223	135	0.01%	0.002%
52	8.786	2398	2409	2436	rBV	368109	618985	67.83%	9.089%
53	9.095	2499	2505	2508	rBV2	278	316	0.03%	0.005%
54	9.133	2514	2517	2519	rBV	231	138	0.02%	0.002%
55	9.214	2539	2542	2545	rVB	252	118	0.01%	0.002%
56	9.272	2557	2560	2564	rVB2	234	141	0.02%	0.002%
57	9.664	2677	2682	2683	rBV2	222	127	0.01%	0.002%
58	9.754	2706	2710	2713	rBV3	152	170	0.02%	0.002%
59	9.866	2743	2745	2748	rVB2	216	105	0.01%	0.002%
60	9.927	2760	2764	2765	rBV	212	117	0.01%	0.002%
61	9.963	2772	2775	2778	rVB3	300	196	0.02%	0.003%
62	10.156	2817	2835	2856	rBV	259053	408855	44.80%	6.004%
63	10.288	2874	2876	2879	rBV2	261	175	0.02%	0.003%
64	10.329	2881	2889	2901	rVB3	4980	7624	0.84%	0.112%
65	10.490	2935	2939	2944	rVB3	279	251	0.03%	0.004%
66	10.529	2948	2951	2954	rBV2	228	149	0.02%	0.002%
67	10.841	3044	3048	3051	rBV2	172	149	0.02%	0.002%
68	10.870	3054	3057	3060	rBV2	211	127	0.01%	0.002%
69	10.886	3060	3062	3063	rBV	589	277	0.03%	0.004%
70	11.014	3099	3102	3107	rBV3	190	157	0.02%	0.002%
71	11.188	3145	3156	3179	rBV	401371	618375	67.76%	9.080%
72	11.361	3208	3210	3213	rBV2	331	152	0.02%	0.002%
73	11.509	3246	3256	3261	rBV5	3561	6878	0.75%	0.101%
74	11.564	3262	3273	3295	rVB	408259	652792	71.53%	9.586%
75	11.844	3358	3360	3363	rVB	268	113	0.01%	0.002%
76	11.908	3377	3380	3387	rVB3	406	376	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
 Data File : VV032140.D
 Acq On : 20 Sep 2023 12:26
 Operator : SY/MD
 Sample : 04385-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYP5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	11.940	3388	3390	3393	rVB	268	129	0.01%	0.002%
78	11.969	3394	3399	3405	rBV2	313	318	0.03%	0.005%
79	12.194	3465	3469	3470	rBV2	898	543	0.06%	0.008%
80	12.246	3483	3485	3491	rVB2	218	155	0.02%	0.002%
81	12.297	3494	3501	3512	rBV5	2559	3809	0.42%	0.056%
82	12.378	3523	3526	3535	rBV2	343	455	0.05%	0.007%
83	12.442	3543	3546	3549	rBV2	216	136	0.01%	0.002%
84	12.596	3589	3594	3599	rBV3	690	522	0.06%	0.008%
85	12.667	3614	3616	3619	rBV2	317	162	0.02%	0.002%
86	12.821	3661	3664	3667	rVB2	199	108	0.01%	0.002%
87	13.168	3770	3772	3776	rBV3	270	176	0.02%	0.003%
88	13.210	3779	3785	3791	rVB3	1129	1260	0.14%	0.019%
89	13.259	3797	3800	3803	rBV2	211	175	0.02%	0.003%
90	13.323	3817	3820	3826	rBV3	219	233	0.03%	0.003%
91	13.355	3826	3830	3833	rBV2	262	211	0.02%	0.003%
92	13.374	3833	3836	3839	rVB2	303	199	0.02%	0.003%
93	13.394	3839	3842	3844	rBV	238	160	0.02%	0.002%
94	13.451	3853	3860	3868	rBV4	3728	5198	0.57%	0.076%
95	13.596	3903	3905	3906	rBV2	276	116	0.01%	0.002%
96	13.689	3928	3934	3943	rBV5	1364	1833	0.20%	0.027%
97	13.828	3974	3977	3981	rBV2	250	200	0.02%	0.003%
98	13.924	4003	4007	4009	rBV3	384	330	0.04%	0.005%
99	14.188	4084	4089	4090	rBV	205	137	0.02%	0.002%
100	14.599	4215	4217	4219	rBV2	275	105	0.01%	0.002%




Sum of corrected areas: 6810117

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
Data File : VV032140.D
Acq On : 20 Sep 2023 12:26
Operator : SY/MD
Sample : 04385-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYP5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

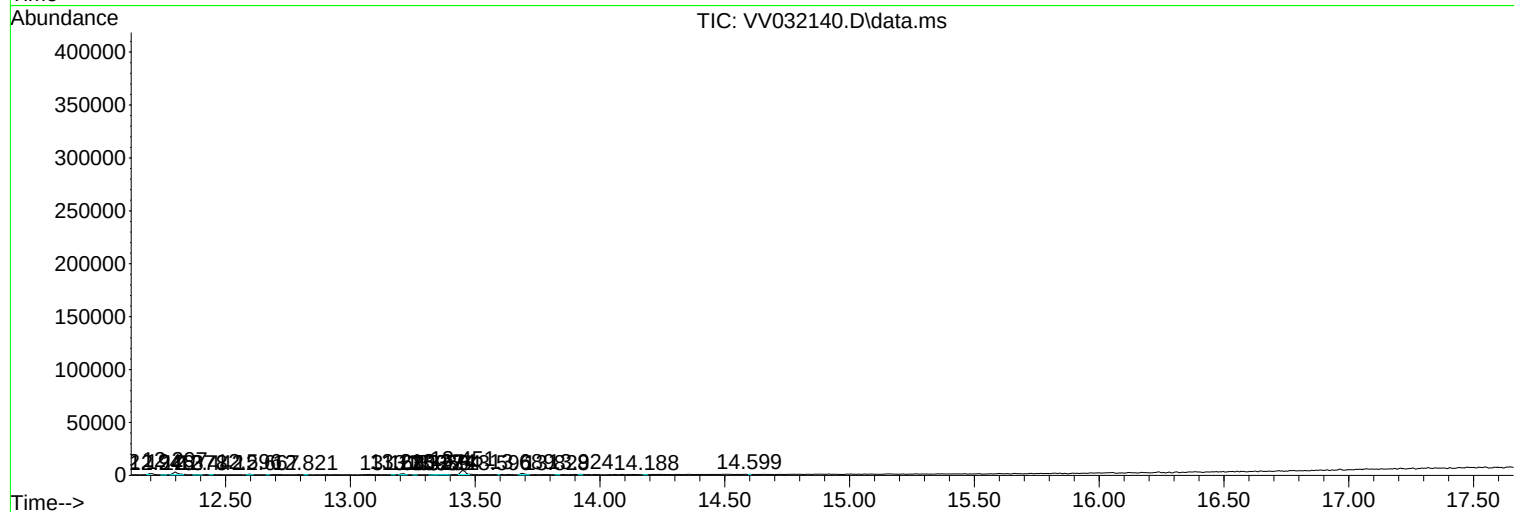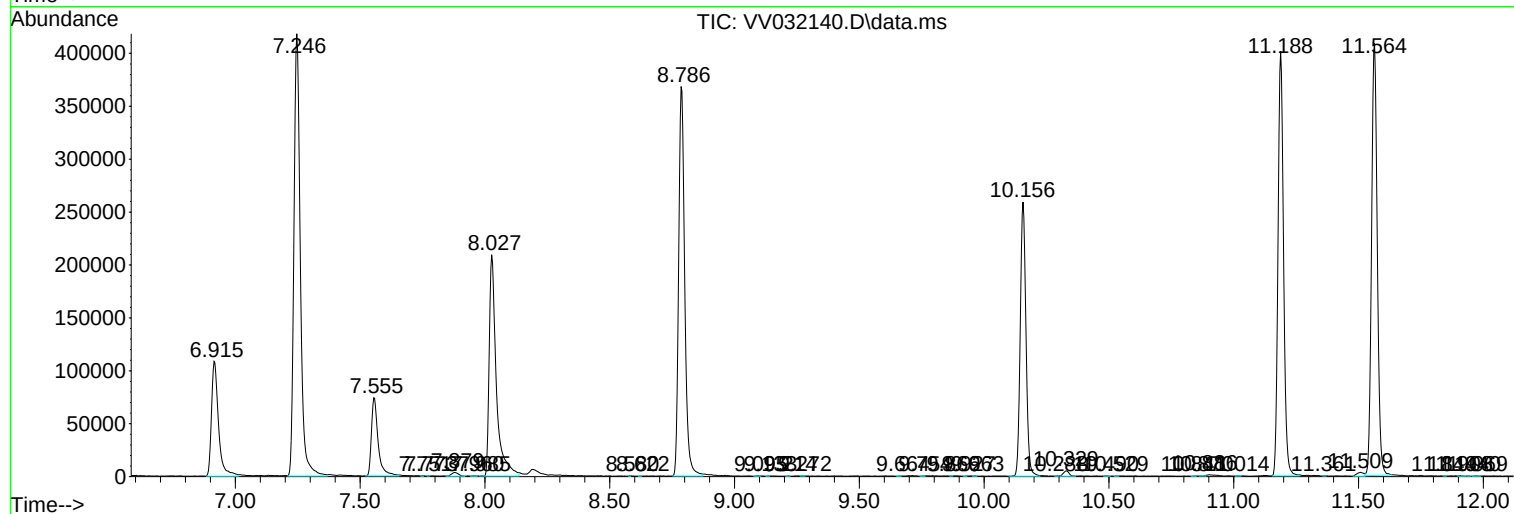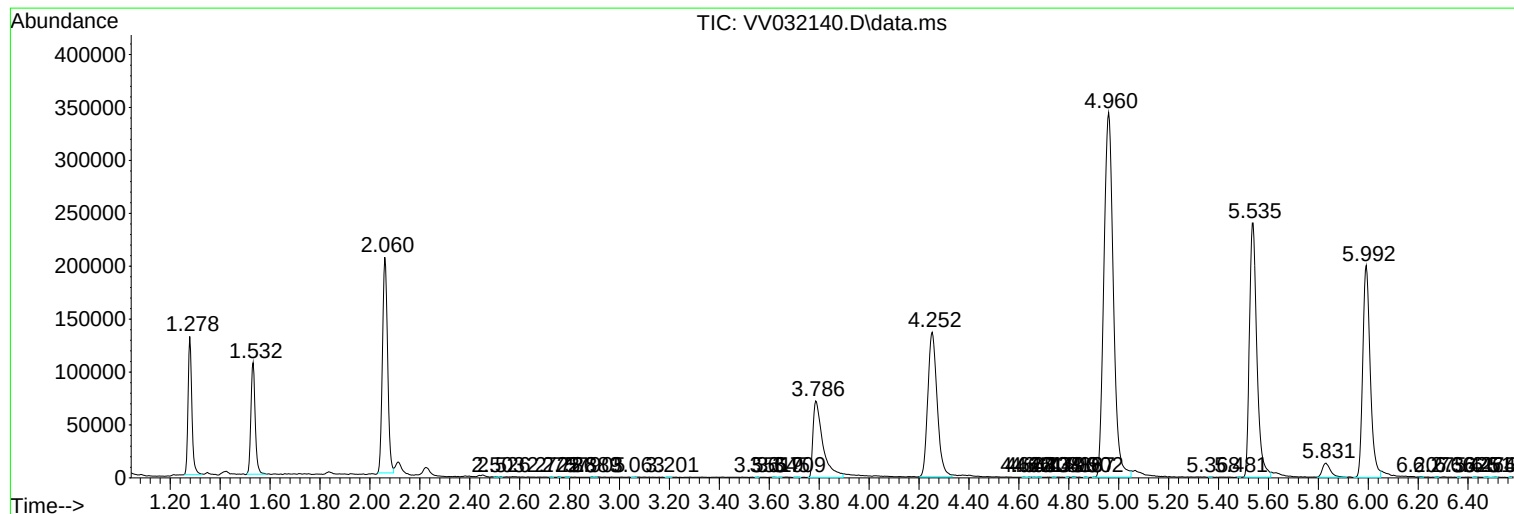

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
Data File : VV032140.D
Acq On : 20 Sep 2023 12:26
Operator : SY/MD
Sample : 04385-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYP5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
Data File : VV032140.D
Acq On : 20 Sep 2023 12:26
Operator : SY/MD
Sample : 04385-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYP5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------