

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
 Data File : VV032141.D
 Acq On : 20 Sep 2023 12:49
 Operator : SY/MD
 Sample : 04385-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYS0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV032141.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	110889	115196	15.03%	1.872%
2	1.532	146	153	171	rVB	90975	108861	14.21%	1.769%
3	2.059	308	317	328	rBV	169844	246893	32.22%	4.012%
4	2.529	459	463	465	rBV3	309	249	0.03%	0.004%
5	2.561	470	473	476	rVV3	327	232	0.03%	0.004%
6	2.693	512	514	517	rVB2	314	141	0.02%	0.002%
7	2.712	517	520	522	rBV2	171	110	0.01%	0.002%
8	2.957	594	596	598	rBV	212	112	0.01%	0.002%
9	2.995	605	608	613	rBV	142	137	0.02%	0.002%
10	3.416	736	739	742	rBV	127	110	0.01%	0.002%
11	3.542	775	778	782	rBV	174	137	0.02%	0.002%
12	3.590	789	793	795	rBV2	140	118	0.02%	0.002%
13	3.699	824	827	830	rBV2	194	134	0.02%	0.002%
14	3.789	846	855	892	rBV	58711	160774	20.98%	2.613%
15	4.252	984	999	1025	rBV	114599	295855	38.61%	4.808%
16	4.590	1101	1104	1106	rBV2	355	244	0.03%	0.004%
17	4.628	1113	1116	1120	rBV2	274	253	0.03%	0.004%
18	4.786	1162	1165	1169	rBV3	220	221	0.03%	0.004%
19	4.825	1173	1177	1181	rVB3	326	231	0.03%	0.004%
20	4.960	1202	1219	1247	rBV2	291684	766307	100.00%	12.454%
21	5.336	1334	1336	1339	rBV	256	166	0.02%	0.003%
22	5.538	1387	1399	1422	rBV	262959	545314	71.16%	8.862%
23	5.831	1478	1490	1506	rBV2	12581	26759	3.49%	0.435%
24	5.992	1526	1540	1576	rBV	166151	356148	46.48%	5.788%
25	6.278	1624	1629	1633	rBV5	435	505	0.07%	0.008%
26	6.390	1661	1664	1667	rBV2	210	158	0.02%	0.003%
27	6.461	1684	1686	1693	rVB	295	189	0.02%	0.003%
28	6.503	1694	1699	1702	rBV2	260	249	0.03%	0.004%
29	6.654	1741	1746	1749	rVB	453	396	0.05%	0.006%
30	6.725	1763	1768	1771	rBV2	333	273	0.04%	0.004%
31	6.747	1771	1775	1778	rBV	278	205	0.03%	0.003%
32	6.841	1796	1804	1805	rBV2	241	201	0.03%	0.003%
33	6.918	1817	1828	1857	rBV	89459	175339	22.88%	2.850%
34	7.246	1919	1930	1964	rBV	345348	619421	80.83%	10.067%
35	7.554	2017	2026	2049	rBV	60227	113700	14.84%	1.848%
36	7.879	2118	2127	2136	rBV4	1344	2204	0.29%	0.036%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
 Data File : VV032141.D
 Acq On : 20 Sep 2023 12:49
 Operator : SY/MD
 Sample : 04385-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYS0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	7.953	2148	2150	2155	rVB2	308	200	0.03%	0.003%
38	7.979	2155	2158	2160	rVB	256	121	0.02%	0.002%
39	8.030	2163	2174	2218	rBV	169759	347737	45.38%	5.651%
40	8.509	2320	2323	2326	rBV2	269	214	0.03%	0.003%
41	8.542	2329	2333	2335	rBV2	304	227	0.03%	0.004%
42	8.567	2340	2341	2347	rBV2	268	169	0.02%	0.003%
43	8.599	2349	2351	2355	rVB2	230	131	0.02%	0.002%
44	8.625	2355	2359	2364	rBV2	338	318	0.04%	0.005%
45	8.648	2364	2366	2373	rVB2	193	133	0.02%	0.002%
46	8.699	2379	2382	2386	rVB2	322	236	0.03%	0.004%
47	8.744	2392	2396	2398	rBV	415	231	0.03%	0.004%
48	8.786	2398	2409	2441	rBV	403943	679276	88.64%	11.039%
49	8.953	2459	2461	2465	rVB3	457	218	0.03%	0.004%
50	8.998	2473	2475	2477	rBV2	272	141	0.02%	0.002%
51	9.030	2484	2485	2490	rVB	295	165	0.02%	0.003%
52	9.226	2542	2546	2548	rBV2	191	120	0.02%	0.002%
53	9.493	2625	2629	2631	rBV	263	152	0.02%	0.002%
54	9.532	2638	2641	2644	rVV2	258	175	0.02%	0.003%
55	9.689	2685	2690	2693	rBV3	325	343	0.04%	0.006%
56	9.734	2701	2704	2705	rBV	341	151	0.02%	0.002%
57	9.763	2710	2713	2715	rBV2	258	175	0.02%	0.003%
58	9.821	2726	2731	2732	rBV	273	168	0.02%	0.003%
59	9.857	2738	2742	2743	rBV	261	142	0.02%	0.002%
60	9.882	2749	2750	2754	rVB2	271	159	0.02%	0.003%
61	9.985	2777	2782	2787	rBV	179	238	0.03%	0.004%
62	10.156	2821	2835	2854	rBV	210897	339119	44.25%	5.511%
63	10.297	2876	2879	2881	rBV2	201	118	0.02%	0.002%
64	10.323	2881	2887	2888	rBV4	1624	1209	0.16%	0.020%
65	10.493	2936	2940	2942	rVB2	264	149	0.02%	0.002%
66	10.519	2943	2948	2950	rBV2	233	208	0.03%	0.003%
67	10.821	3040	3042	3048	rBV2	310	222	0.03%	0.004%
68	10.902	3060	3067	3069	rBV3	864	1009	0.13%	0.016%
69	11.040	3107	3110	3112	rBV3	214	155	0.02%	0.003%
70	11.088	3122	3125	3130	rBV3	176	214	0.03%	0.003%
71	11.114	3130	3133	3136	rBV3	436	283	0.04%	0.005%
72	11.130	3136	3138	3142	rVB	436	259	0.03%	0.004%
73	11.188	3142	3156	3181	rBV	445367	681802	88.97%	11.080%
74	11.387	3214	3218	3223	rVB2	359	356	0.05%	0.006%
75	11.416	3223	3227	3231	rBV2	161	185	0.02%	0.003%
76	11.500	3247	3253	3254	rBV3	2694	2130	0.28%	0.035%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
 Data File : VV032141.D
 Acq On : 20 Sep 2023 12:49
 Operator : SY/MD
 Sample : 04385-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYS0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	11.564	3262	3273	3292	rVB	348000	544389	71.04%	8.847%
78	11.747	3327	3330	3333	rBV2	144	115	0.02%	0.002%
79	11.850	3359	3362	3366	rVB2	251	193	0.03%	0.003%
80	11.998	3406	3408	3411	rVB	398	209	0.03%	0.003%
81	12.030	3416	3418	3422	rVB	396	199	0.03%	0.003%
82	12.053	3422	3425	3430	rBV	189	221	0.03%	0.004%
83	12.107	3440	3442	3450	rVB2	315	239	0.03%	0.004%
84	12.188	3465	3467	3470	rBV	499	416	0.05%	0.007%
85	12.300	3493	3502	3506	rBV6	2549	3590	0.47%	0.058%
86	12.339	3512	3514	3516	rBV2	286	118	0.02%	0.002%
87	12.426	3539	3541	3543	rVB	278	111	0.01%	0.002%
88	12.593	3589	3593	3598	rBV2	396	459	0.06%	0.007%
89	12.882	3681	3683	3690	rBV2	223	192	0.03%	0.003%
90	13.024	3724	3727	3731	rVB2	295	181	0.02%	0.003%
91	13.094	3746	3749	3756	rVB3	416	301	0.04%	0.005%
92	13.204	3779	3783	3788	rBV4	540	546	0.07%	0.009%
93	13.451	3852	3860	3873	rBV2	2332	3745	0.49%	0.061%
94	13.561	3892	3894	3896	rBV	204	122	0.02%	0.002%
95	13.590	3899	3903	3908	rBV2	325	330	0.04%	0.005%
96	13.683	3929	3932	3935	rBV2	540	480	0.06%	0.008%
97	13.734	3946	3948	3952	rVB2	237	134	0.02%	0.002%
98	13.834	3975	3979	3984	rBV4	390	323	0.04%	0.005%
99	13.953	4014	4016	4017	rBV	289	112	0.01%	0.002%
100	14.184	4085	4088	4091	rVB2	301	182	0.02%	0.003%




Sum of corrected areas: 6153207

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
Data File : VV032141.D
Acq On : 20 Sep 2023 12:49
Operator : SY/MD
Sample : 04385-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYS0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

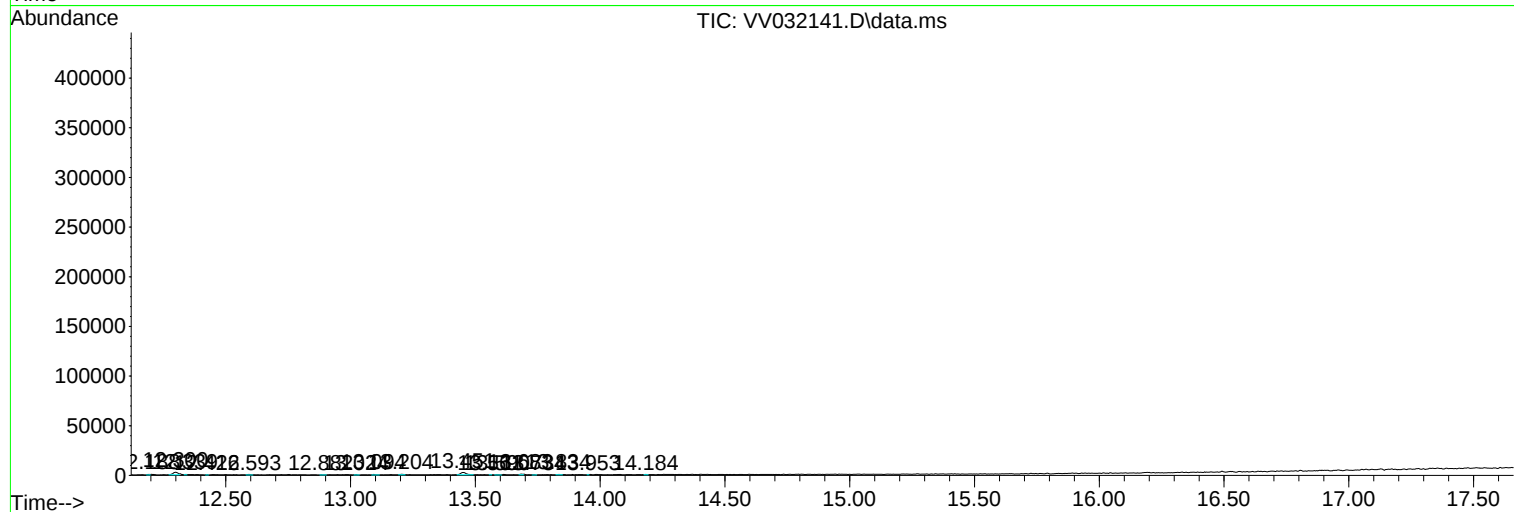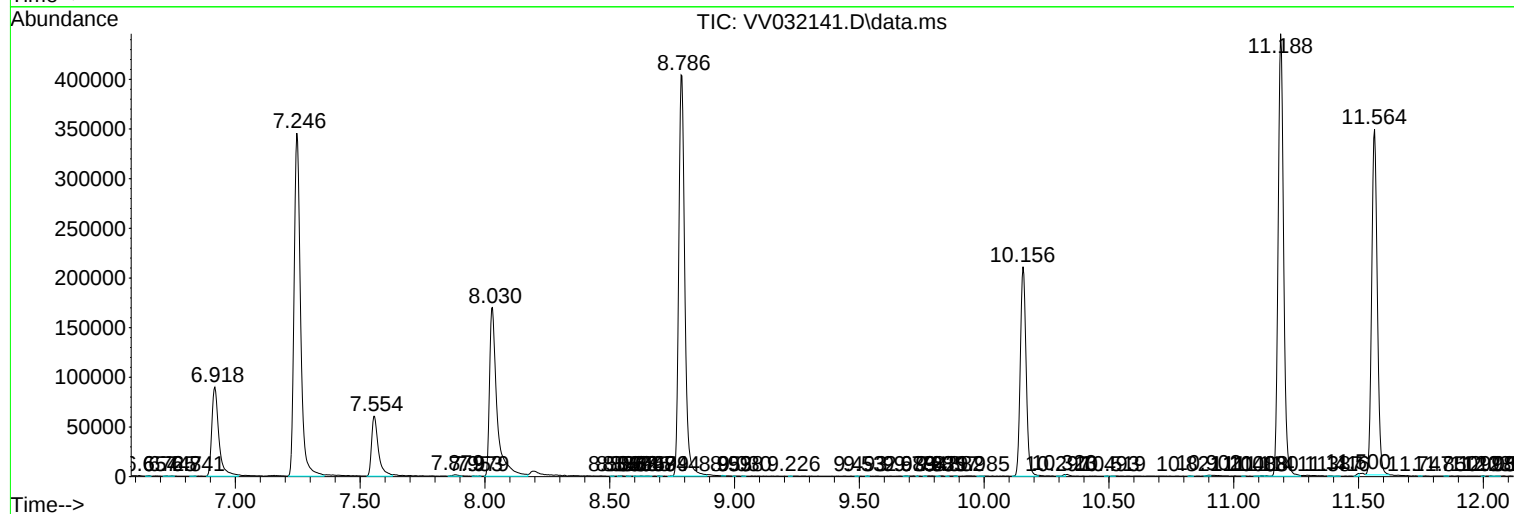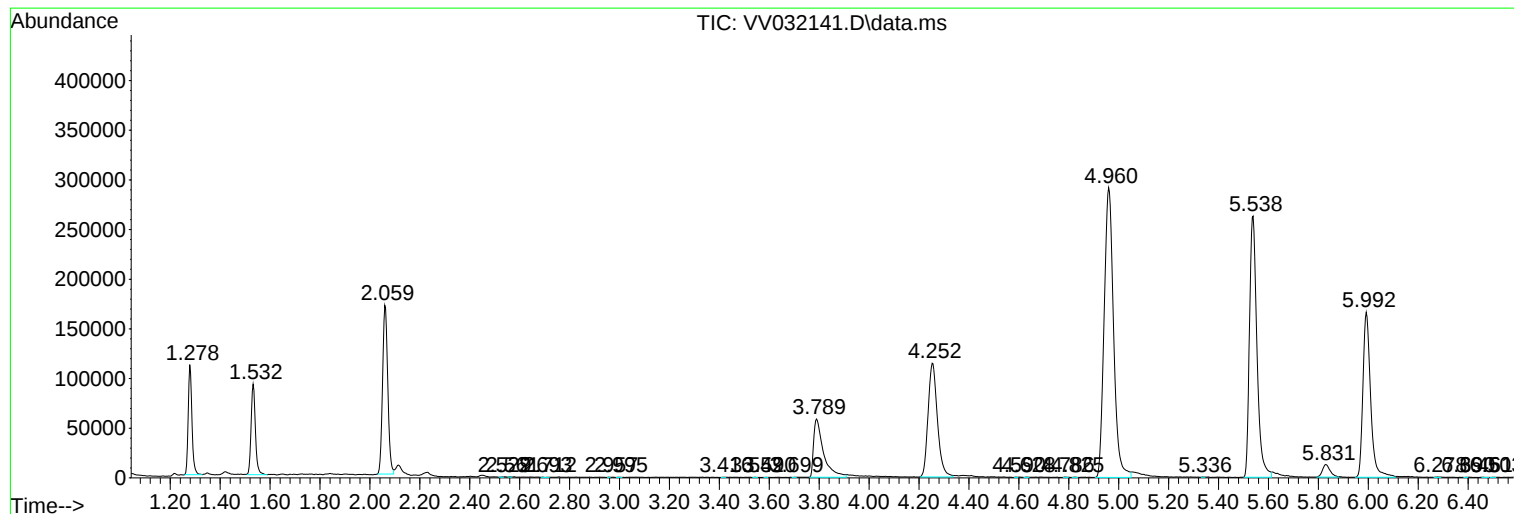

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
Data File : VV032141.D
Acq On : 20 Sep 2023 12:49
Operator : SY/MD
Sample : 04385-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYS0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
Data File : VV032141.D
Acq On : 20 Sep 2023 12:49
Operator : SY/MD
Sample : 04385-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYS0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------