

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
 Data File : VV032143.D
 Acq On : 20 Sep 2023 13:36
 Operator : SY/MD
 Sample : 04417-19ME
 Misc : 4.83g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYX1ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV032143.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.185	41	45	50	rBV	5968	5185	0.68%	0.094%
2	1.278	67	74	100	rVB	64200	109300	14.41%	1.973%
3	2.034	300	309	329	rVB	148620	218555	28.81%	3.946%
4	2.654	499	502	505	rVB3	384	226	0.03%	0.004%
5	2.670	505	507	510	rBV2	345	180	0.02%	0.003%
6	2.770	535	538	544	rBV2	184	264	0.03%	0.005%
7	2.822	551	554	555	rBV	186	90	0.01%	0.002%
8	2.944	585	592	593	rBV4	959	1022	0.13%	0.018%
9	3.027	615	618	619	rBV	234	156	0.02%	0.003%
10	3.053	624	626	629	rVB	200	113	0.01%	0.002%
11	3.133	648	651	652	rBV	136	82	0.01%	0.001%
12	3.191	666	669	672	rVB3	222	148	0.02%	0.003%
13	3.207	672	674	677	rBV	289	129	0.02%	0.002%
14	3.278	694	696	700	rVB2	177	89	0.01%	0.002%
15	3.358	717	721	724	rBV	221	210	0.03%	0.004%
16	3.410	734	737	739	rBV	128	88	0.01%	0.002%
17	3.461	750	753	755	rBV2	233	151	0.02%	0.003%
18	3.519	761	771	774	rBV2	274	349	0.05%	0.006%
19	3.654	811	813	816	rVB	273	84	0.01%	0.002%
20	3.728	834	836	840	rVB2	206	101	0.01%	0.002%
21	3.754	841	844	849	rVB2	238	148	0.02%	0.003%
22	3.809	852	861	894	rBV	36459	125625	16.56%	2.268%
23	4.249	982	998	1025	rBV2	95129	261005	34.41%	4.712%
24	4.567	1088	1097	1099	rBV4	876	895	0.12%	0.016%
25	4.622	1112	1114	1115	rBV4	212	110	0.01%	0.002%
26	4.674	1128	1130	1133	rVB3	209	90	0.01%	0.002%
27	4.760	1153	1157	1161	rBV2	222	176	0.02%	0.003%
28	4.780	1161	1163	1167	rVB2	176	105	0.01%	0.002%
29	4.831	1176	1179	1181	rBV2	267	171	0.02%	0.003%
30	4.876	1191	1193	1196	rBV2	283	212	0.03%	0.004%
31	4.953	1201	1217	1249	rBV2	267800	675628	89.07%	12.198%
32	5.159	1279	1281	1284	rBV2	291	200	0.03%	0.004%
33	5.246	1306	1308	1310	rVB	370	128	0.02%	0.002%
34	5.387	1347	1352	1356	rBV3	322	299	0.04%	0.005%
35	5.532	1386	1397	1428	rBV	263766	575033	75.81%	10.382%
36	5.770	1469	1471	1474	rVB2	362	170	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
 Data File : VV032143.D
 Acq On : 20 Sep 2023 13:36
 Operator : SY/MD
 Sample : 04417-19ME
 Misc : 4.83g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYX1ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	5.834	1479	1491	1509	rBV8	8416	21326	2.81%	0.385%
38	5.992	1528	1540	1569	rVB	139682	311253	41.03%	5.620%
39	6.198	1602	1604	1607	rBV	363	251	0.03%	0.005%
40	6.301	1633	1636	1638	rVB	182	83	0.01%	0.001%
41	6.365	1652	1656	1666	rBV3	226	305	0.04%	0.006%
42	6.410	1667	1670	1672	rBV2	227	119	0.02%	0.002%
43	6.426	1673	1675	1680	rVB2	248	147	0.02%	0.003%
44	6.487	1691	1694	1701	rVB2	118	122	0.02%	0.002%
45	6.516	1701	1703	1704	rBV2	225	105	0.01%	0.002%
46	6.551	1712	1714	1716	rBV2	245	122	0.02%	0.002%
47	6.580	1721	1723	1724	rBV	247	79	0.01%	0.001%
48	6.606	1729	1731	1733	rBV3	223	148	0.02%	0.003%
49	6.690	1754	1757	1759	rBV2	217	152	0.02%	0.003%
50	6.702	1759	1761	1764	rBV	223	186	0.02%	0.003%
51	6.850	1801	1807	1813	rBV3	493	557	0.07%	0.010%
52	6.879	1813	1816	1817	rBV	273	171	0.02%	0.003%
53	6.918	1817	1828	1853	rBV	75930	155571	20.51%	2.809%
54	7.079	1875	1878	1884	rVB2	405	353	0.05%	0.006%
55	7.143	1896	1898	1899	rBV	275	112	0.01%	0.002%
56	7.194	1911	1914	1916	rBV	269	158	0.02%	0.003%
57	7.246	1918	1930	1960	rBV	299589	546679	72.07%	9.870%
58	7.558	2017	2027	2057	rBV	50487	105518	13.91%	1.905%
59	7.802	2101	2103	2107	rVB2	284	204	0.03%	0.004%
60	7.834	2111	2113	2114	rBV	149	81	0.01%	0.001%
61	7.844	2114	2116	2118	rVB	364	122	0.02%	0.002%
62	7.911	2134	2137	2140	rBV2	370	246	0.03%	0.004%
63	8.005	2162	2166	2167	rBV2	229	156	0.02%	0.003%
64	8.043	2167	2178	2179	rBV	81023	100553	13.26%	1.815%
65	8.358	2274	2276	2279	rBV2	369	130	0.02%	0.002%
66	8.583	2344	2346	2348	rBV	166	88	0.01%	0.002%
67	8.599	2348	2351	2354	rBV3	557	394	0.05%	0.007%
68	8.648	2364	2366	2369	rBV	195	152	0.02%	0.003%
69	8.683	2372	2377	2379	rBV3	182	155	0.02%	0.003%
70	8.789	2397	2410	2433	rBV	406039	721052	95.06%	13.019%
71	9.056	2491	2493	2497	rVB2	251	155	0.02%	0.003%
72	9.095	2497	2505	2507	rBV3	1274	1674	0.22%	0.030%
73	9.217	2535	2543	2547	rBV2	250	293	0.04%	0.005%
74	9.352	2582	2585	2587	rBV	232	116	0.02%	0.002%
75	9.423	2605	2607	2611	rVB3	300	189	0.02%	0.003%
76	9.452	2612	2616	2621	rBV2	205	248	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
 Data File : VV032143.D
 Acq On : 20 Sep 2023 13:36
 Operator : SY/MD
 Sample : 04417-19ME
 Misc : 4.83g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYX1ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	9.497	2625	2630	2637	rVB4	699	949	0.13%	0.017%
78	9.651	2674	2678	2679	rBV3	772	530	0.07%	0.010%
79	9.696	2687	2692	2695	rBV2	136	128	0.02%	0.002%
80	9.712	2695	2697	2701	rVB	204	81	0.01%	0.001%
81	9.741	2701	2706	2708	rBV2	567	497	0.07%	0.009%
82	9.844	2737	2738	2741	rVB	259	78	0.01%	0.001%
83	9.869	2741	2746	2749	rBV3	329	328	0.04%	0.006%
84	9.886	2749	2751	2755	rVB2	399	168	0.02%	0.003%
85	9.915	2758	2760	2761	rBV	260	106	0.01%	0.002%
86	9.966	2767	2776	2783	rBV2	694	1153	0.15%	0.021%
87	10.005	2783	2788	2789	rBV2	220	132	0.02%	0.002%
88	10.098	2814	2817	2822	rBV2	184	146	0.02%	0.003%
89	10.162	2822	2837	2857	rBV	176352	313049	41.27%	5.652%
90	10.268	2868	2870	2872	rBV3	388	160	0.02%	0.003%
91	10.297	2876	2879	2880	rBV	222	140	0.02%	0.003%
92	10.381	2902	2905	2906	rBV2	280	127	0.02%	0.002%
93	10.400	2907	2911	2913	rVV2	449	280	0.04%	0.005%
94	10.442	2922	2924	2925	rBV	480	135	0.02%	0.002%
95	10.487	2936	2938	2939	rBV	445	189	0.02%	0.003%
96	10.525	2943	2950	2962	rVB4	2768	4862	0.64%	0.088%
97	10.612	2975	2977	2980	rVB2	605	290	0.04%	0.005%
98	10.979	3084	3091	3096	rBV4	1252	1853	0.24%	0.033%
99	11.191	3146	3157	3178	rBV	473906	758544	100.00%	13.696%
100	11.567	3263	3274	3296	rBV	317655	508653	67.06%	9.184%




Sum of corrected areas: 5538620

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
Data File : VV032143.D
Acq On : 20 Sep 2023 13:36
Operator : SY/MD
Sample : 04417-19ME
Misc : 4.83g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYX1ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

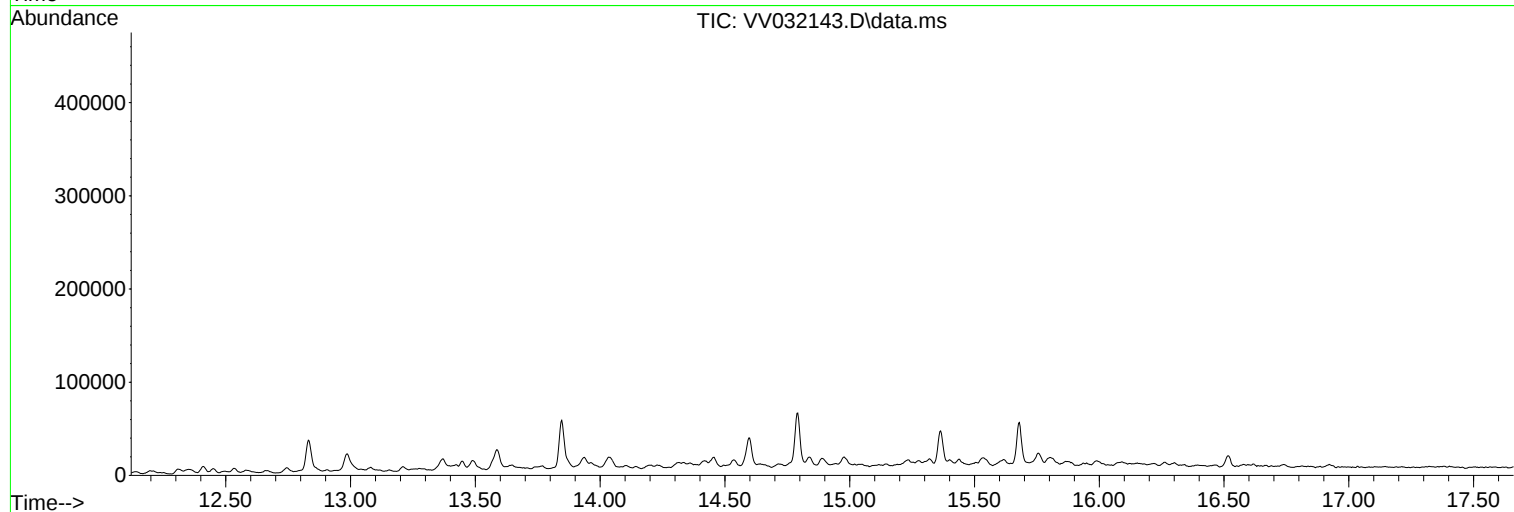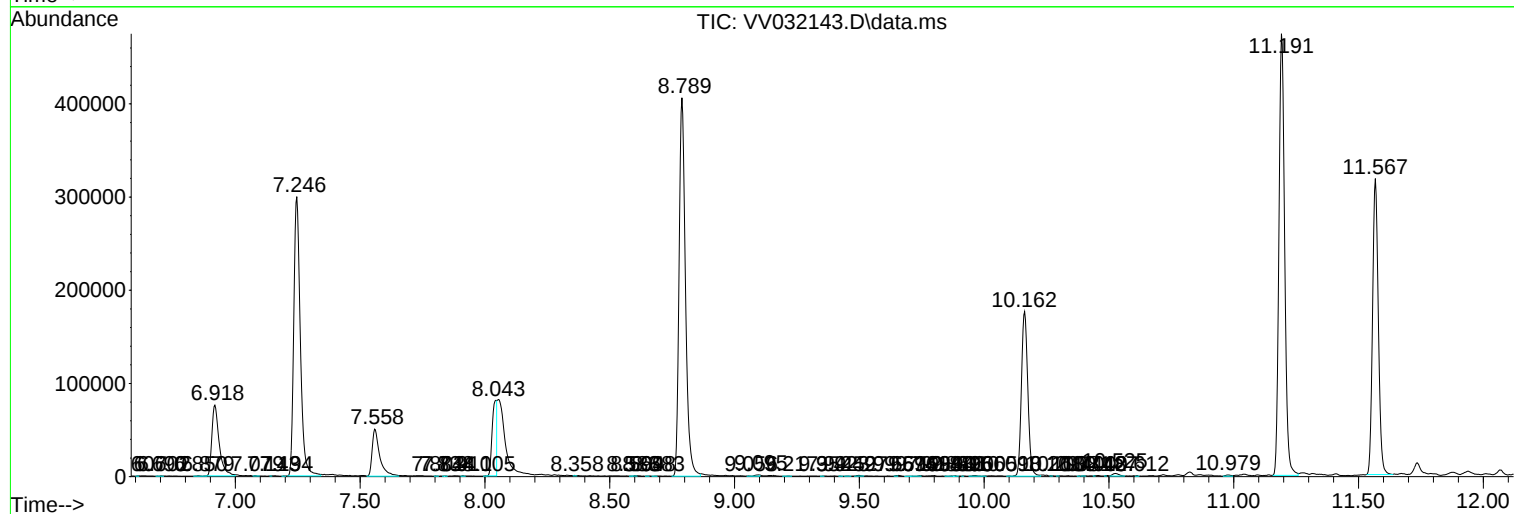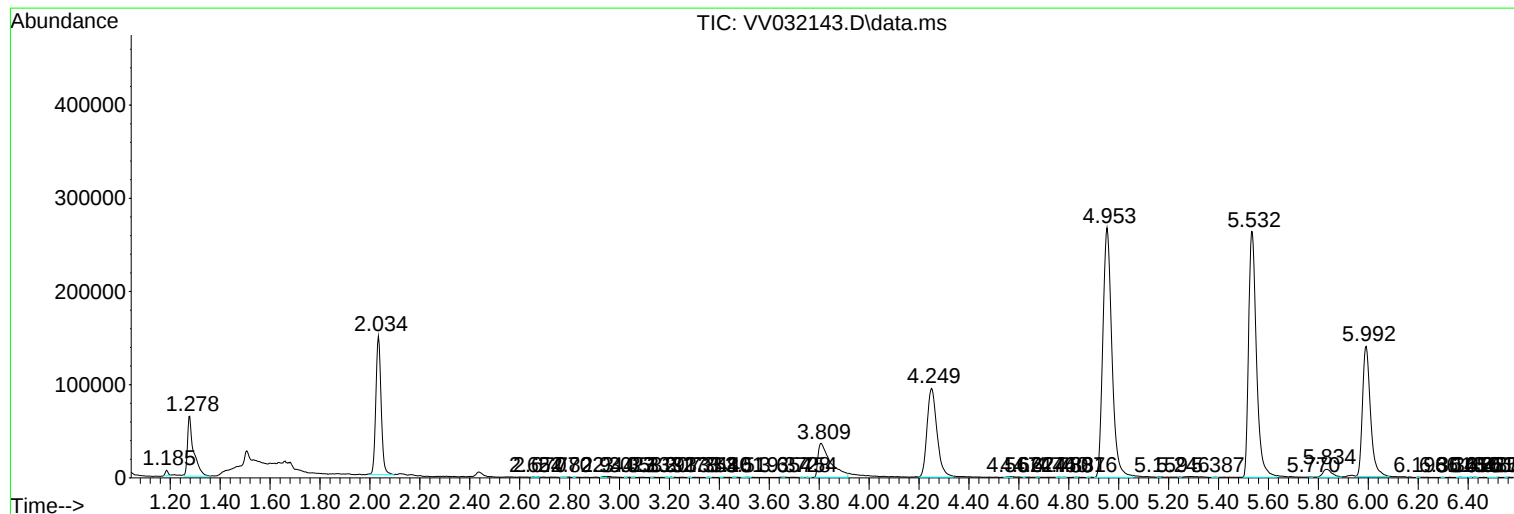

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
Data File : VV032143.D
Acq On : 20 Sep 2023 13:36
Operator : SY/MD
Sample : 04417-19ME
Misc : 4.83g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYX1ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
Data File : VV032143.D
Acq On : 20 Sep 2023 13:36
Operator : SY/MD
Sample : 04417-19ME
Misc : 4.83g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYX1ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc