

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
 Data File : VV032144.D
 Acq On : 20 Sep 2023 13:59
 Operator : SY/MD
 Sample : 04417-05ME
 Misc : 4.43g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYF4ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV032144.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.185	40	45	50	rBV	7109	6743	0.83%	0.113%
2	1.278	67	74	97	rVB	72160	109667	13.48%	1.834%
3	2.037	301	310	325	rVB	149171	217557	26.74%	3.639%
4	2.683	509	511	514	rVB	324	158	0.02%	0.003%
5	2.741	526	529	535	rBV2	401	384	0.05%	0.006%
6	2.834	555	558	559	rBV	305	156	0.02%	0.003%
7	2.844	559	561	565	rVB	374	243	0.03%	0.004%
8	2.953	587	595	605	rVB5	1381	2723	0.33%	0.046%
9	3.088	633	637	640	rVB2	173	157	0.02%	0.003%
10	3.307	703	705	709	rVB3	303	159	0.02%	0.003%
11	3.432	741	744	747	rBV	229	169	0.02%	0.003%
12	3.619	799	802	806	rVB	224	144	0.02%	0.002%
13	3.805	852	860	906	rBV	38049	136778	16.81%	2.288%
14	4.249	982	998	1023	rBV	98636	265380	32.61%	4.438%
15	4.574	1096	1099	1101	rVV2	355	161	0.02%	0.003%
16	4.587	1101	1103	1105	rVB3	345	173	0.02%	0.003%
17	4.616	1109	1112	1115	rBV2	234	184	0.02%	0.003%
18	4.632	1115	1117	1120	rVB2	272	147	0.02%	0.002%
19	4.696	1134	1137	1141	rVB2	229	152	0.02%	0.003%
20	4.767	1156	1159	1162	rBV2	259	150	0.02%	0.003%
21	4.818	1171	1175	1180	rBV2	330	286	0.04%	0.005%
22	4.953	1202	1217	1252	rBV2	273591	697722	85.75%	11.669%
23	5.378	1348	1349	1352	rVB	451	206	0.03%	0.003%
24	5.535	1385	1398	1428	rBV	282366	610083	74.98%	10.204%
25	5.831	1479	1490	1510	rBV7	7979	19850	2.44%	0.332%
26	5.992	1529	1540	1562	rVB	143914	309495	38.04%	5.176%
27	6.133	1580	1584	1589	rBV6	867	994	0.12%	0.017%
28	6.182	1598	1599	1602	rVB2	424	152	0.02%	0.003%
29	6.223	1608	1612	1613	rBV	295	180	0.02%	0.003%
30	6.246	1616	1619	1624	rVB2	481	314	0.04%	0.005%
31	6.313	1637	1640	1642	rBV	253	147	0.02%	0.002%
32	6.538	1704	1710	1711	rBV	146	144	0.02%	0.002%
33	6.600	1726	1729	1732	rVV2	395	268	0.03%	0.004%
34	6.619	1733	1735	1737	rBV2	460	195	0.02%	0.003%
35	6.735	1769	1771	1774	rVB2	348	176	0.02%	0.003%
36	6.764	1777	1780	1783	rBV2	413	200	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
 Data File : VV032144.D
 Acq On : 20 Sep 2023 13:59
 Operator : SY/MD
 Sample : 04417-05ME
 Misc : 4.43g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYF4ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	6.837	1799	1803	1804	rBV	215	185	0.02%	0.003%
38	6.918	1817	1828	1853	rBV	78950	162430	19.96%	2.717%
39	7.143	1896	1898	1901	rBV3	537	304	0.04%	0.005%
40	7.191	1912	1913	1916	rBV3	207	141	0.02%	0.002%
41	7.246	1918	1930	1953	rBV	312826	566140	69.58%	9.469%
42	7.558	2017	2027	2057	rBV	51674	109767	13.49%	1.836%
43	7.780	2092	2096	2101	rBV2	313	342	0.04%	0.006%
44	7.837	2113	2114	2118	rVB2	329	154	0.02%	0.003%
45	7.992	2157	2162	2166	rBV2	348	321	0.04%	0.005%
46	8.053	2166	2181	2207	rBV	94526	288968	35.51%	4.833%
47	8.464	2307	2309	2310	rBV	474	207	0.03%	0.003%
48	8.497	2317	2319	2322	rVB3	369	181	0.02%	0.003%
49	8.522	2322	2327	2330	rBV2	417	344	0.04%	0.006%
50	8.564	2338	2340	2345	rBV2	415	255	0.03%	0.004%
51	8.606	2349	2353	2356	rBV4	336	309	0.04%	0.005%
52	8.680	2372	2376	2378	rBV2	272	197	0.02%	0.003%
53	8.718	2387	2388	2391	rBV2	283	190	0.02%	0.003%
54	8.789	2398	2410	2440	rBV	427741	764989	94.02%	12.794%
55	9.339	2578	2581	2585	rVB2	255	200	0.02%	0.003%
56	9.371	2585	2591	2593	rBV	246	199	0.02%	0.003%
57	9.439	2609	2612	2615	rVB	515	277	0.03%	0.005%
58	9.632	2670	2672	2676	rBV	275	151	0.02%	0.003%
59	9.783	2717	2719	2723	rVB3	364	247	0.03%	0.004%
60	9.808	2723	2727	2729	rBV2	251	159	0.02%	0.003%
61	9.953	2766	2772	2773	rBV4	362	275	0.03%	0.005%
62	10.005	2786	2788	2793	rVV2	273	294	0.04%	0.005%
63	10.024	2793	2794	2799	rVV2	361	294	0.04%	0.005%
64	10.050	2799	2802	2803	rVV	266	163	0.02%	0.003%
65	10.069	2806	2808	2815	rVB2	381	212	0.03%	0.004%
66	10.162	2824	2837	2856	rBV	189727	321149	39.47%	5.371%
67	10.316	2883	2885	2889	rBV2	311	198	0.02%	0.003%
68	10.461	2928	2930	2934	rVB2	236	146	0.02%	0.002%
69	10.487	2934	2938	2939	rBV	209	163	0.02%	0.003%
70	10.532	2946	2952	2959	rVB4	1195	1612	0.20%	0.027%
71	10.657	2990	2991	2994	rBV2	366	235	0.03%	0.004%
72	10.779	3022	3029	3032	rBV3	828	902	0.11%	0.015%
73	10.857	3049	3053	3057	rBV4	518	488	0.06%	0.008%
74	10.947	3078	3081	3083	rBV	322	172	0.02%	0.003%
75	11.191	3146	3157	3183	rBV	516522	813678	100.00%	13.609%
76	11.567	3262	3274	3293	rBV	339027	531199	65.28%	8.884%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
 Data File : VV032144.D
 Acq On : 20 Sep 2023 13:59
 Operator : SY/MD
 Sample : 04417-05ME
 Misc : 4.43g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYF4ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	11.789	3339	3343	3346	rBV	593	430	0.05%	0.007%
78	11.824	3351	3354	3356	rBV2	428	227	0.03%	0.004%
79	11.857	3361	3364	3367	rVB	323	178	0.02%	0.003%
80	11.931	3380	3387	3388	rBV3	429	388	0.05%	0.006%
81	11.995	3405	3407	3410	rBV3	297	197	0.02%	0.003%
82	12.017	3412	3414	3417	rVB2	408	196	0.02%	0.003%
83	12.066	3427	3429	3432	rBV	304	226	0.03%	0.004%
84	12.082	3432	3434	3437	rVB2	373	176	0.02%	0.003%
85	12.246	3481	3485	3494	rVB4	483	668	0.08%	0.011%
86	12.304	3494	3503	3505	rBV3	712	659	0.08%	0.011%
87	12.316	3505	3507	3512	rVB3	564	294	0.04%	0.005%
88	12.487	3558	3560	3564	rVB3	342	233	0.03%	0.004%
89	12.532	3571	3574	3575	rBV2	311	213	0.03%	0.004%
90	12.574	3583	3587	3589	rBV2	308	256	0.03%	0.004%
91	12.728	3634	3635	3637	rBV	382	187	0.02%	0.003%
92	12.908	3684	3691	3693	rBV4	469	494	0.06%	0.008%
93	12.924	3693	3696	3698	rBV	275	189	0.02%	0.003%
94	13.075	3740	3743	3748	rBV5	572	670	0.08%	0.011%
95	13.194	3778	3780	3782	rBV	378	172	0.02%	0.003%
96	13.246	3792	3796	3799	rBV2	629	610	0.07%	0.010%
97	13.278	3802	3806	3809	rBV2	305	304	0.04%	0.005%
98	13.808	3967	3971	3974	rBV5	677	701	0.09%	0.012%
99	14.599	4207	4217	4225	rBV9	4050	7675	0.94%	0.128%
100	14.792	4263	4277	4284	rBV4	8089	14150	1.74%	0.237%




Sum of corrected areas: 5979127

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
Data File : VV032144.D
Acq On : 20 Sep 2023 13:59
Operator : SY/MD
Sample : 04417-05ME
Misc : 4.43g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYF4ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

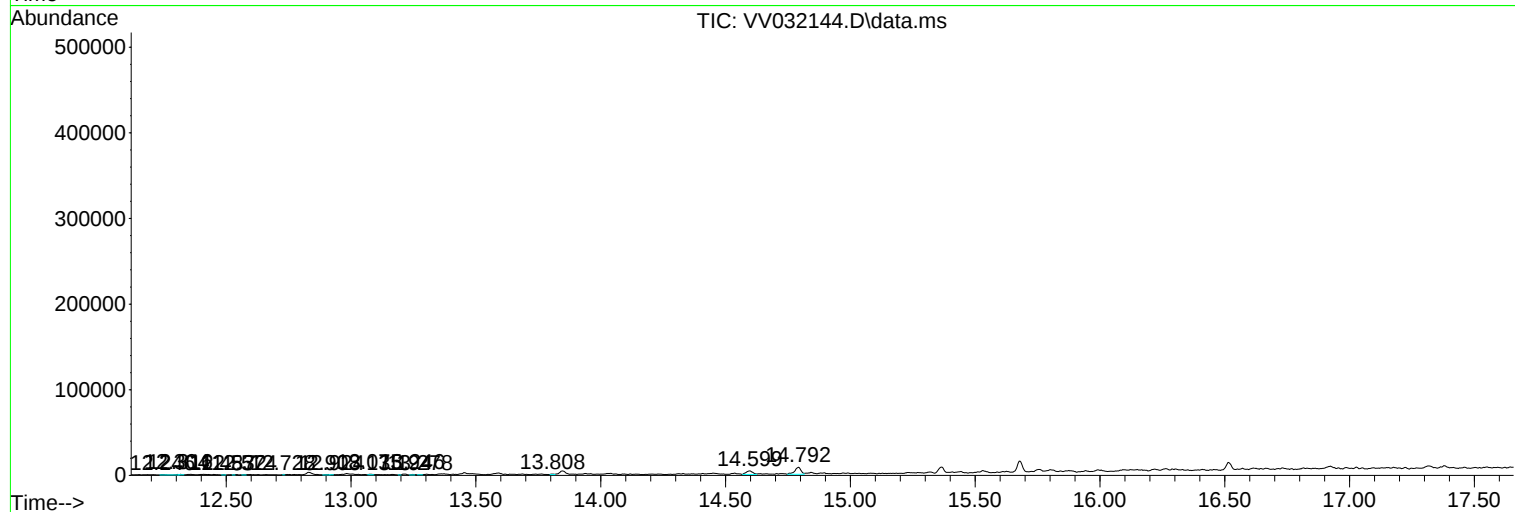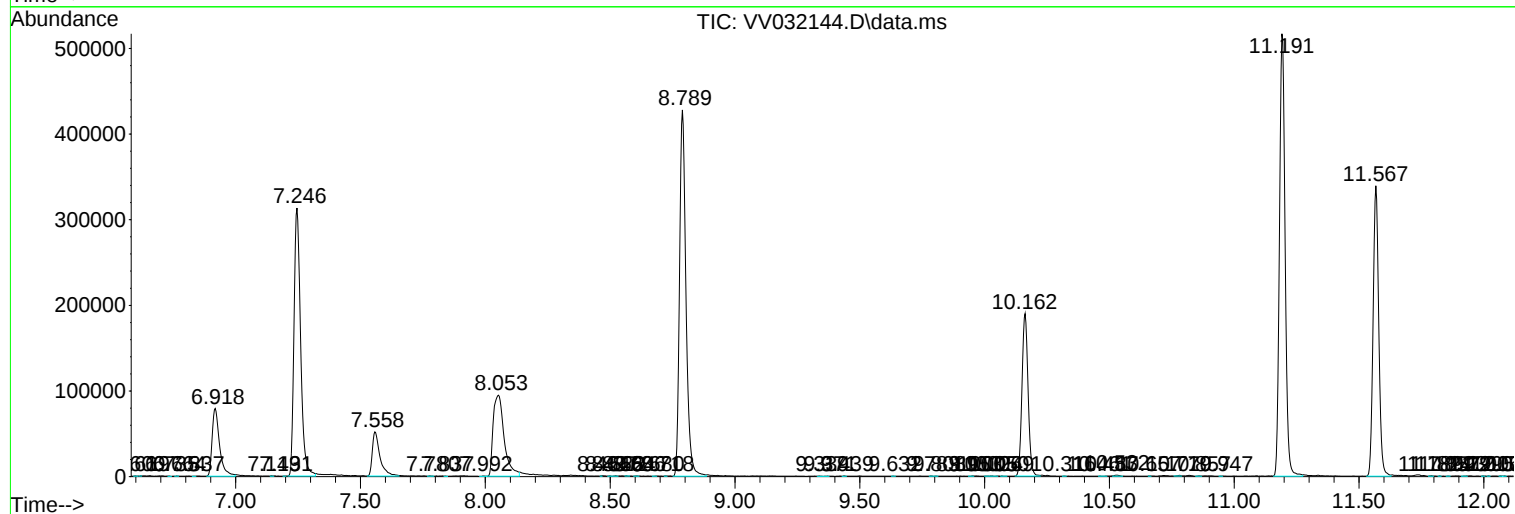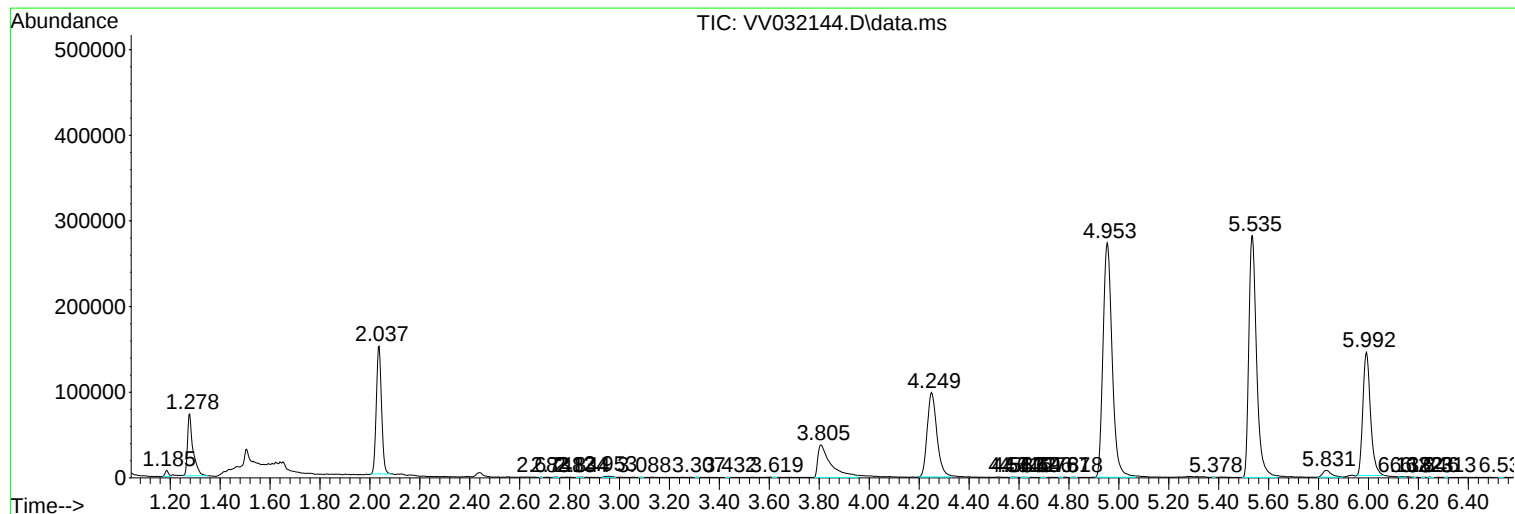

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
Data File : VV032144.D
Acq On : 20 Sep 2023 13:59
Operator : SY/MD
Sample : 04417-05ME
Misc : 4.43g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYF4ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
Data File : VV032144.D
Acq On : 20 Sep 2023 13:59
Operator : SY/MD
Sample : 04417-05ME
Misc : 4.43g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYF4ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc