

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
 Data File : VV032145.D
 Acq On : 20 Sep 2023 14:23
 Operator : SY/MD
 Sample : 04417-23ME
 Misc : 5.64g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EYZE7ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV032145.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.185	40	45	50	rBV2	7894	7415	0.91%	0.124%
2	1.275	67	73	89	rBV	69744	103573	12.72%	1.730%
3	2.037	301	310	330	rVB	149824	221085	27.15%	3.692%
4	2.654	499	502	503	rBV	394	212	0.03%	0.004%
5	2.799	545	547	550	rVB2	382	151	0.02%	0.003%
6	2.892	574	576	579	rBV	327	161	0.02%	0.003%
7	2.953	587	595	607	rBV5	1249	2964	0.36%	0.049%
8	3.150	654	656	662	rVB2	299	175	0.02%	0.003%
9	3.207	670	674	677	rBV2	220	171	0.02%	0.003%
10	3.577	787	789	792	rVB	247	119	0.01%	0.002%
11	3.642	803	809	812	rBV3	448	496	0.06%	0.008%
12	3.773	841	850	851	rBV3	256	218	0.03%	0.004%
13	3.806	851	860	898	rBV2	39016	134302	16.49%	2.243%
14	4.249	980	998	1029	rBV	99164	270184	33.18%	4.512%
15	4.506	1076	1078	1082	rBV	175	126	0.02%	0.002%
16	4.568	1091	1097	1100	rBV5	1279	1608	0.20%	0.027%
17	4.651	1119	1123	1124	rBV3	336	241	0.03%	0.004%
18	4.738	1148	1150	1152	rVV2	236	117	0.01%	0.002%
19	4.754	1152	1155	1158	rVV2	222	141	0.02%	0.002%
20	4.786	1161	1165	1167	rVB2	266	205	0.03%	0.003%
21	4.953	1200	1217	1244	rBV2	274932	694152	85.25%	11.592%
22	5.195	1290	1292	1294	rBV2	384	222	0.03%	0.004%
23	5.349	1338	1340	1342	rBV	335	158	0.02%	0.003%
24	5.474	1377	1379	1381	rVB	319	136	0.02%	0.002%
25	5.490	1381	1384	1385	rBV2	203	116	0.01%	0.002%
26	5.532	1385	1397	1427	rBV	279164	601601	73.88%	10.047%
27	5.831	1479	1490	1504	rBV3	8370	20339	2.50%	0.340%
28	5.989	1528	1539	1567	rVB	143212	316887	38.92%	5.292%
29	6.214	1608	1609	1612	rVB2	248	135	0.02%	0.002%
30	6.233	1612	1615	1616	rBV2	217	129	0.02%	0.002%
31	6.259	1621	1623	1625	rBV	367	137	0.02%	0.002%
32	6.381	1656	1661	1665	rBV3	464	333	0.04%	0.006%
33	6.426	1669	1675	1677	rBV	283	177	0.02%	0.003%
34	6.584	1718	1724	1727	rVB3	363	398	0.05%	0.007%
35	6.612	1727	1733	1735	rBV3	862	865	0.11%	0.014%
36	6.664	1744	1749	1753	rVB3	386	273	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
 Data File : VV032145.D
 Acq On : 20 Sep 2023 14:23
 Operator : SY/MD
 Sample : 04417-23ME
 Misc : 5.64g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYE7ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	6.703	1756	1761	1763	rBV2	401	364	0.04%	0.006%
38	6.773	1779	1783	1786	rBV4	404	301	0.04%	0.005%
39	6.850	1802	1807	1812	rBV3	706	817	0.10%	0.014%
40	6.918	1817	1828	1854	rBV2	79902	162513	19.96%	2.714%
41	7.140	1895	1897	1900	rBV3	221	184	0.02%	0.003%
42	7.246	1919	1930	1949	rBV	311737	561694	68.98%	9.380%
43	7.487	2002	2005	2006	rBV	401	236	0.03%	0.004%
44	7.558	2018	2027	2059	rBV	51585	106250	13.05%	1.774%
45	7.805	2102	2104	2106	rBV	233	133	0.02%	0.002%
46	7.828	2109	2111	2113	rVV	334	141	0.02%	0.002%
47	7.873	2121	2125	2126	rBV2	282	183	0.02%	0.003%
48	7.915	2134	2138	2141	rBV3	231	197	0.02%	0.003%
49	8.050	2167	2180	2212	rBV	99662	295494	36.29%	4.935%
50	8.403	2288	2290	2293	rBV2	522	281	0.03%	0.005%
51	8.452	2302	2305	2308	rVB3	579	300	0.04%	0.005%
52	8.474	2308	2312	2314	rBV2	508	397	0.05%	0.007%
53	8.503	2318	2321	2326	rVB2	735	716	0.09%	0.012%
54	8.551	2331	2336	2338	rVV2	271	223	0.03%	0.004%
55	8.564	2338	2340	2344	rVB2	354	188	0.02%	0.003%
56	8.677	2372	2375	2378	rVB2	477	325	0.04%	0.005%
57	8.699	2378	2382	2383	rBV	173	116	0.01%	0.002%
58	8.789	2398	2410	2443	rBV	426877	762405	93.63%	12.732%
59	9.088	2496	2503	2506	rBV4	1774	1827	0.22%	0.031%
60	9.304	2567	2570	2574	rBV2	203	145	0.02%	0.002%
61	9.355	2582	2586	2589	rBV	322	225	0.03%	0.004%
62	9.429	2605	2609	2613	rBV	156	161	0.02%	0.003%
63	9.500	2621	2631	2636	rBV5	1139	1921	0.24%	0.032%
64	9.571	2651	2653	2659	rVB	228	137	0.02%	0.002%
65	9.651	2671	2678	2682	rVB4	506	527	0.06%	0.009%
66	9.683	2682	2688	2693	rVB3	307	292	0.04%	0.005%
67	9.715	2693	2698	2701	rBV3	449	325	0.04%	0.005%
68	9.735	2701	2704	2708	rVB2	512	313	0.04%	0.005%
69	9.760	2708	2712	2715	rBV	349	264	0.03%	0.004%
70	9.792	2717	2722	2729	rVB2	673	746	0.09%	0.012%
71	9.857	2738	2742	2747	rBV2	183	171	0.02%	0.003%
72	9.882	2747	2750	2755	rBV2	543	402	0.05%	0.007%
73	9.950	2764	2771	2772	rBV2	501	411	0.05%	0.007%
74	10.008	2786	2789	2793	rBV3	231	200	0.02%	0.003%
75	10.030	2793	2796	2801	rVV3	258	203	0.02%	0.003%
76	10.063	2801	2806	2810	rVB5	369	377	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
 Data File : VV032145.D
 Acq On : 20 Sep 2023 14:23
 Operator : SY/MD
 Sample : 04417-23ME
 Misc : 5.64g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYE7ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	10.162	2824	2837	2855	rVV	189497	321341	39.46%	5.366%
78	10.394	2906	2909	2913	rBV2	404	208	0.03%	0.003%
79	10.464	2927	2931	2932	rBV2	255	173	0.02%	0.003%
80	10.484	2933	2937	2941	rVV4	609	622	0.08%	0.010%
81	10.526	2946	2950	2960	rVB7	1954	2898	0.36%	0.048%
82	10.593	2969	2971	2973	rVB	388	133	0.02%	0.002%
83	10.712	3006	3008	3009	rBV	331	116	0.01%	0.002%
84	10.963	3082	3086	3089	rBV2	198	113	0.01%	0.002%
85	10.989	3092	3094	3095	rBV2	228	111	0.01%	0.002%
86	11.046	3109	3112	3116	rBV2	232	225	0.03%	0.004%
87	11.091	3125	3126	3129	rBV	450	212	0.03%	0.004%
88	11.191	3146	3157	3180	rBV	520580	814267	100.00%	13.598%
89	11.374	3211	3214	3216	rBV2	319	203	0.02%	0.003%
90	11.464	3238	3242	3244	rVB3	252	144	0.02%	0.002%
91	11.497	3249	3252	3256	rBV2	438	301	0.04%	0.005%
92	11.567	3262	3274	3295	rBV	337418	535985	65.82%	8.951%
93	11.738	3319	3327	3333	rBV2	3881	5245	0.64%	0.088%
94	12.005	3408	3410	3413	rBV3	382	169	0.02%	0.003%
95	12.021	3413	3415	3419	rVB2	617	374	0.05%	0.006%
96	12.056	3422	3426	3427	rBV2	552	412	0.05%	0.007%
97	12.239	3482	3483	3486	rBV2	377	185	0.02%	0.003%
98	12.252	3486	3487	3489	rBV	310	149	0.02%	0.002%
99	12.310	3498	3505	3511	rBV6	1331	2152	0.26%	0.036%
100	12.831	3660	3667	3681	rVB4	14576	20532	2.52%	0.343%




Sum of corrected areas: 5988097

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
Data File : VV032145.D
Acq On : 20 Sep 2023 14:23
Operator : SY/MD
Sample : 04417-23ME
Misc : 5.64g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZY7ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

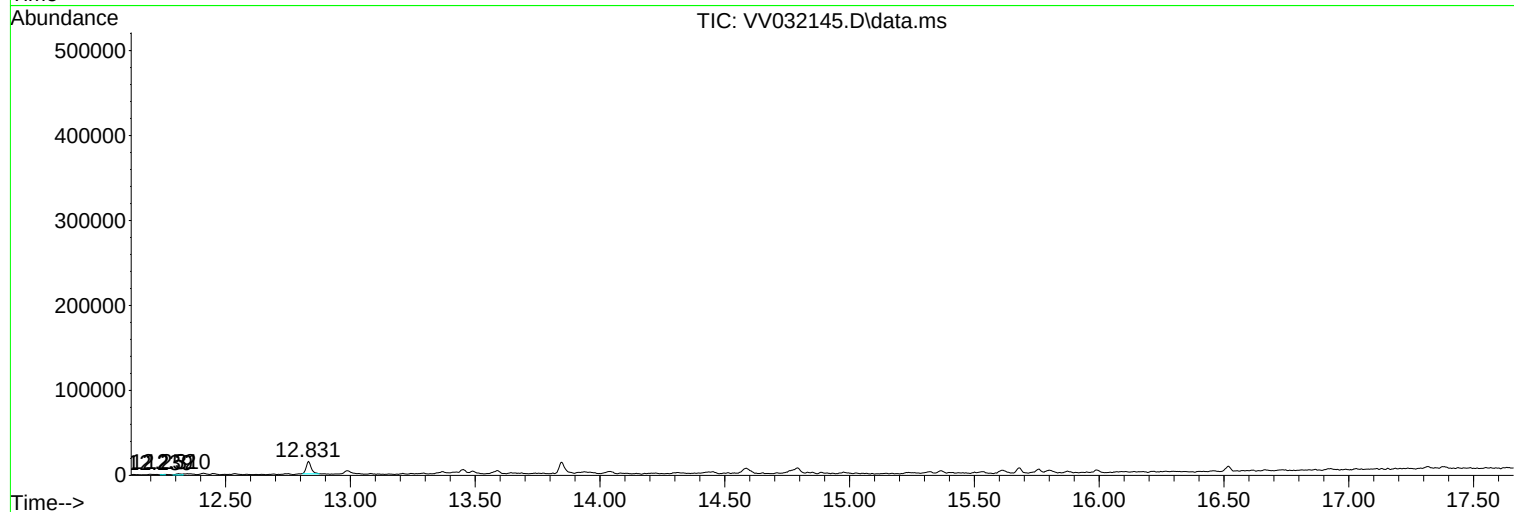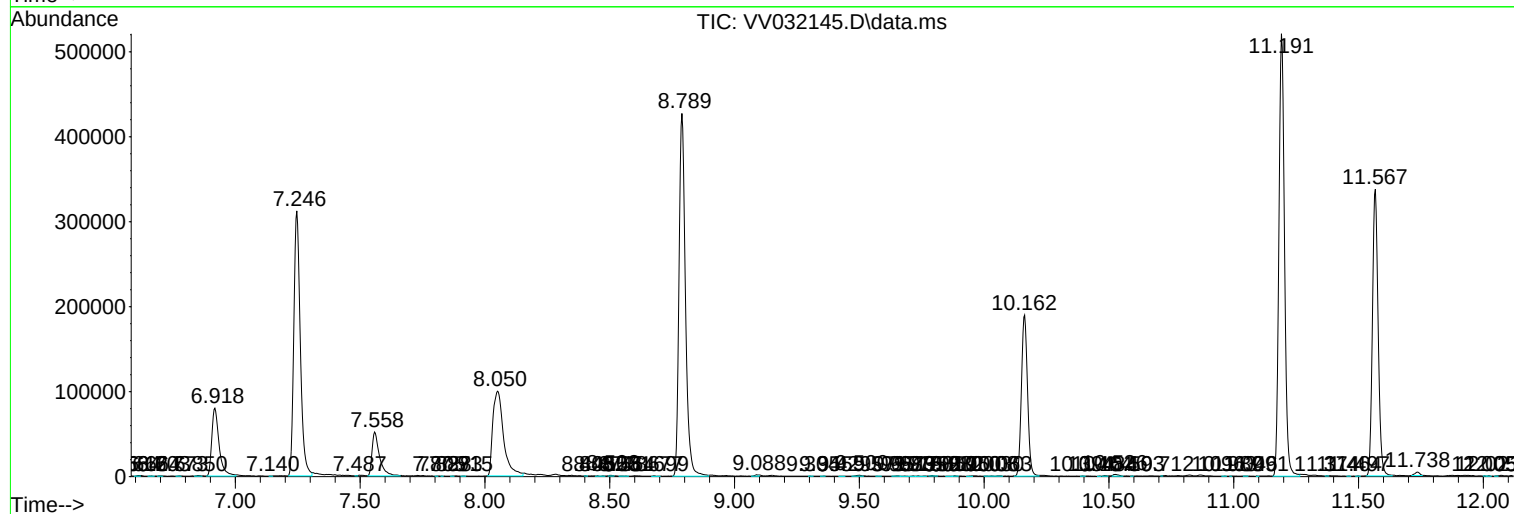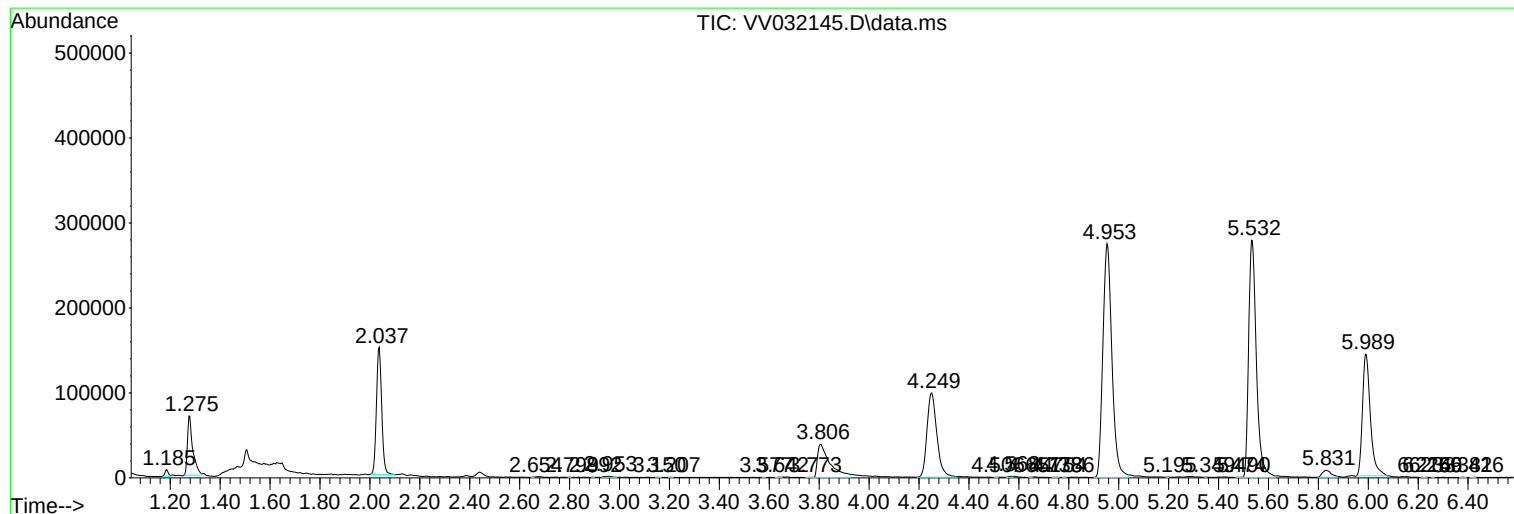

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
Data File : VV032145.D
Acq On : 20 Sep 2023 14:23
Operator : SY/MD
Sample : 04417-23ME
Misc : 5.64g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZY7ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
Data File : VV032145.D
Acq On : 20 Sep 2023 14:23
Operator : SY/MD
Sample : 04417-23ME
Misc : 5.64g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYE7ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc