

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
 Data File : VV032150.D
 Acq On : 20 Sep 2023 16:19
 Operator : SY/MD
 Sample : 04386-22
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK003

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV032150.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	51	55	61	rBV2	2320	2569	0.33%	0.041%
2	1.278	68	74	89	rVB	94399	96174	12.43%	1.549%
3	1.532	146	153	167	rVB	81286	95722	12.37%	1.542%
4	2.060	308	317	328	rBV	145120	208021	26.89%	3.351%
5	2.449	432	438	447	rVB4	4037	6268	0.81%	0.101%
6	2.809	546	550	553	rBV2	184	145	0.02%	0.002%
7	2.918	582	584	585	rBV	260	124	0.02%	0.002%
8	2.969	598	600	607	rVB	313	322	0.04%	0.005%
9	3.018	612	615	619	rBV	120	130	0.02%	0.002%
10	3.201	670	672	677	rBV2	270	154	0.02%	0.002%
11	3.281	695	697	703	rVB2	287	185	0.02%	0.003%
12	3.336	711	714	719	rBV2	138	126	0.02%	0.002%
13	3.362	719	722	726	rVB	246	168	0.02%	0.003%
14	3.715	829	832	836	rBV	513	337	0.04%	0.005%
15	3.789	844	855	885	rBV	63571	171262	22.14%	2.759%
16	4.252	984	999	1027	rBV	114513	297058	38.40%	4.785%
17	4.577	1098	1100	1102	rBV	320	191	0.02%	0.003%
18	4.699	1136	1138	1146	rVV2	266	274	0.04%	0.004%
19	4.770	1154	1160	1165	rBV2	172	200	0.03%	0.003%
20	4.860	1184	1188	1189	rBV	351	170	0.02%	0.003%
21	4.960	1202	1219	1245	rBV2	292963	773534	100.00%	12.461%
22	5.223	1298	1301	1302	rBV2	439	230	0.03%	0.004%
23	5.259	1311	1312	1314	rBV2	262	114	0.01%	0.002%
24	5.368	1345	1346	1350	rVB2	233	148	0.02%	0.002%
25	5.429	1364	1365	1370	rVB3	228	167	0.02%	0.003%
26	5.539	1386	1399	1424	rBV	261663	544591	70.40%	8.773%
27	5.831	1479	1490	1507	rBV3	11740	25894	3.35%	0.417%
28	5.992	1526	1540	1580	rBV	169262	363409	46.98%	5.854%
29	6.284	1629	1631	1634	rVB2	351	200	0.03%	0.003%
30	6.317	1638	1641	1644	rBV2	272	205	0.03%	0.003%
31	6.336	1644	1647	1649	rVB	251	164	0.02%	0.003%
32	6.474	1685	1690	1693	rBV	491	396	0.05%	0.006%
33	6.506	1698	1700	1702	rVB	224	113	0.01%	0.002%
34	6.526	1702	1706	1712	rVB	218	160	0.02%	0.003%
35	6.558	1713	1716	1720	rBV	208	168	0.02%	0.003%
36	6.680	1750	1754	1756	rBV2	322	257	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
 Data File : VV032150.D
 Acq On : 20 Sep 2023 16:19
 Operator : SY/MD
 Sample : 04386-22
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK003

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	6.754	1772	1777	1778	rBV2	181	119	0.02%	0.002%
38	6.789	1784	1788	1791	rBV2	154	143	0.02%	0.002%
39	6.918	1817	1828	1864	rVV	90632	179969	23.27%	2.899%
40	7.185	1909	1911	1914	rBV	202	118	0.02%	0.002%
41	7.246	1918	1930	1968	rBV	334040	608333	78.64%	9.800%
42	7.558	2017	2027	2050	rBV	61892	117638	15.21%	1.895%
43	7.722	2075	2078	2084	rBV3	273	225	0.03%	0.004%
44	7.776	2093	2095	2099	rVB	305	152	0.02%	0.002%
45	7.876	2119	2126	2127	rBV	489	411	0.05%	0.007%
46	7.982	2154	2159	2164	rBV4	1351	1465	0.19%	0.024%
47	8.030	2164	2174	2218	rBV	188364	374932	48.47%	6.040%
48	8.371	2279	2280	2283	rVB	331	128	0.02%	0.002%
49	8.464	2307	2309	2312	rBV	233	158	0.02%	0.003%
50	8.542	2330	2333	2334	rBV2	156	116	0.01%	0.002%
51	8.551	2334	2336	2337	rVV2	293	124	0.02%	0.002%
52	8.599	2347	2351	2352	rBV	246	171	0.02%	0.003%
53	8.622	2353	2358	2361	rVV3	356	309	0.04%	0.005%
54	8.725	2386	2390	2392	rBV2	236	179	0.02%	0.003%
55	8.789	2398	2410	2445	rBV	405379	679792	87.88%	10.951%
56	8.966	2462	2465	2468	rVB3	560	315	0.04%	0.005%
57	9.008	2475	2478	2481	rBV2	269	181	0.02%	0.003%
58	9.053	2490	2492	2494	rBV	333	163	0.02%	0.003%
59	9.075	2495	2499	2502	rBV3	168	177	0.02%	0.003%
60	9.140	2516	2519	2521	rBV2	191	126	0.02%	0.002%
61	9.265	2553	2558	2559	rBV	176	114	0.01%	0.002%
62	9.329	2576	2578	2582	rBV	171	122	0.02%	0.002%
63	9.355	2583	2586	2588	rVV	231	117	0.02%	0.002%
64	9.452	2613	2616	2620	rBV2	129	122	0.02%	0.002%
65	9.500	2626	2631	2635	rVB4	390	426	0.06%	0.007%
66	9.664	2678	2682	2684	rBV	198	171	0.02%	0.003%
67	9.751	2707	2709	2713	rBV3	314	278	0.04%	0.004%
68	9.792	2716	2722	2732	rVB3	659	1237	0.16%	0.020%
69	9.934	2761	2766	2769	rBV3	292	360	0.05%	0.006%
70	9.992	2780	2784	2790	rVB2	307	290	0.04%	0.005%
71	10.030	2790	2796	2798	rBV4	512	538	0.07%	0.009%
72	10.156	2823	2835	2859	rBV	233913	369026	47.71%	5.945%
73	10.278	2870	2873	2880	rVB3	275	271	0.04%	0.004%
74	10.326	2883	2888	2896	rVB4	910	1168	0.15%	0.019%
75	10.397	2907	2910	2913	rVB3	317	192	0.02%	0.003%
76	10.439	2920	2923	2924	rBV2	350	196	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
 Data File : VV032150.D
 Acq On : 20 Sep 2023 16:19
 Operator : SY/MD
 Sample : 04386-22
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK003

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	10.509	2943	2945	2948	rBV2	298	203	0.03%	0.003%
78	10.622	2976	2980	2985	rBV	181	141	0.02%	0.002%
79	10.799	3033	3035	3036	rBV2	257	134	0.02%	0.002%
80	10.815	3036	3040	3041	rBV2	870	628	0.08%	0.010%
81	10.992	3094	3095	3100	rVB4	329	212	0.03%	0.003%
82	11.024	3100	3105	3108	rBV2	522	471	0.06%	0.008%
83	11.043	3108	3111	3113	rBV2	347	186	0.02%	0.003%
84	11.091	3123	3126	3127	rBV2	994	635	0.08%	0.010%
85	11.188	3145	3156	3179	rBV	449861	695772	89.95%	11.209%
86	11.387	3214	3218	3219	rBV2	426	315	0.04%	0.005%
87	11.416	3225	3227	3231	rVB2	408	262	0.03%	0.004%
88	11.435	3231	3233	3237	rBV2	236	137	0.02%	0.002%
89	11.477	3242	3246	3247	rBV	271	190	0.02%	0.003%
90	11.506	3248	3255	3260	rBV5	2654	4204	0.54%	0.068%
91	11.564	3263	3273	3290	rVB	355141	553864	71.60%	8.922%
92	11.866	3361	3367	3369	rBV5	915	914	0.12%	0.015%
93	12.197	3460	3470	3481	rBV7	1794	3355	0.43%	0.054%
94	12.307	3495	3504	3514	rBV8	3972	7424	0.96%	0.120%
95	12.824	3658	3665	3679	rBV8	2468	4767	0.62%	0.077%
96	13.210	3783	3785	3787	rBV2	747	388	0.05%	0.006%
97	13.275	3803	3805	3810	rBV4	735	487	0.06%	0.008%
98	13.303	3812	3814	3815	rBV	387	131	0.02%	0.002%
99	13.564	3890	3895	3896	rBV4	970	870	0.11%	0.014%
100	13.847	3977	3983	3991	rBV9	1538	2410	0.31%	0.039%


Sum of corrected areas: 6207522

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
Data File : VV032150.D
Acq On : 20 Sep 2023 16:19
Operator : SY/MD
Sample : 04386-22
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK003

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

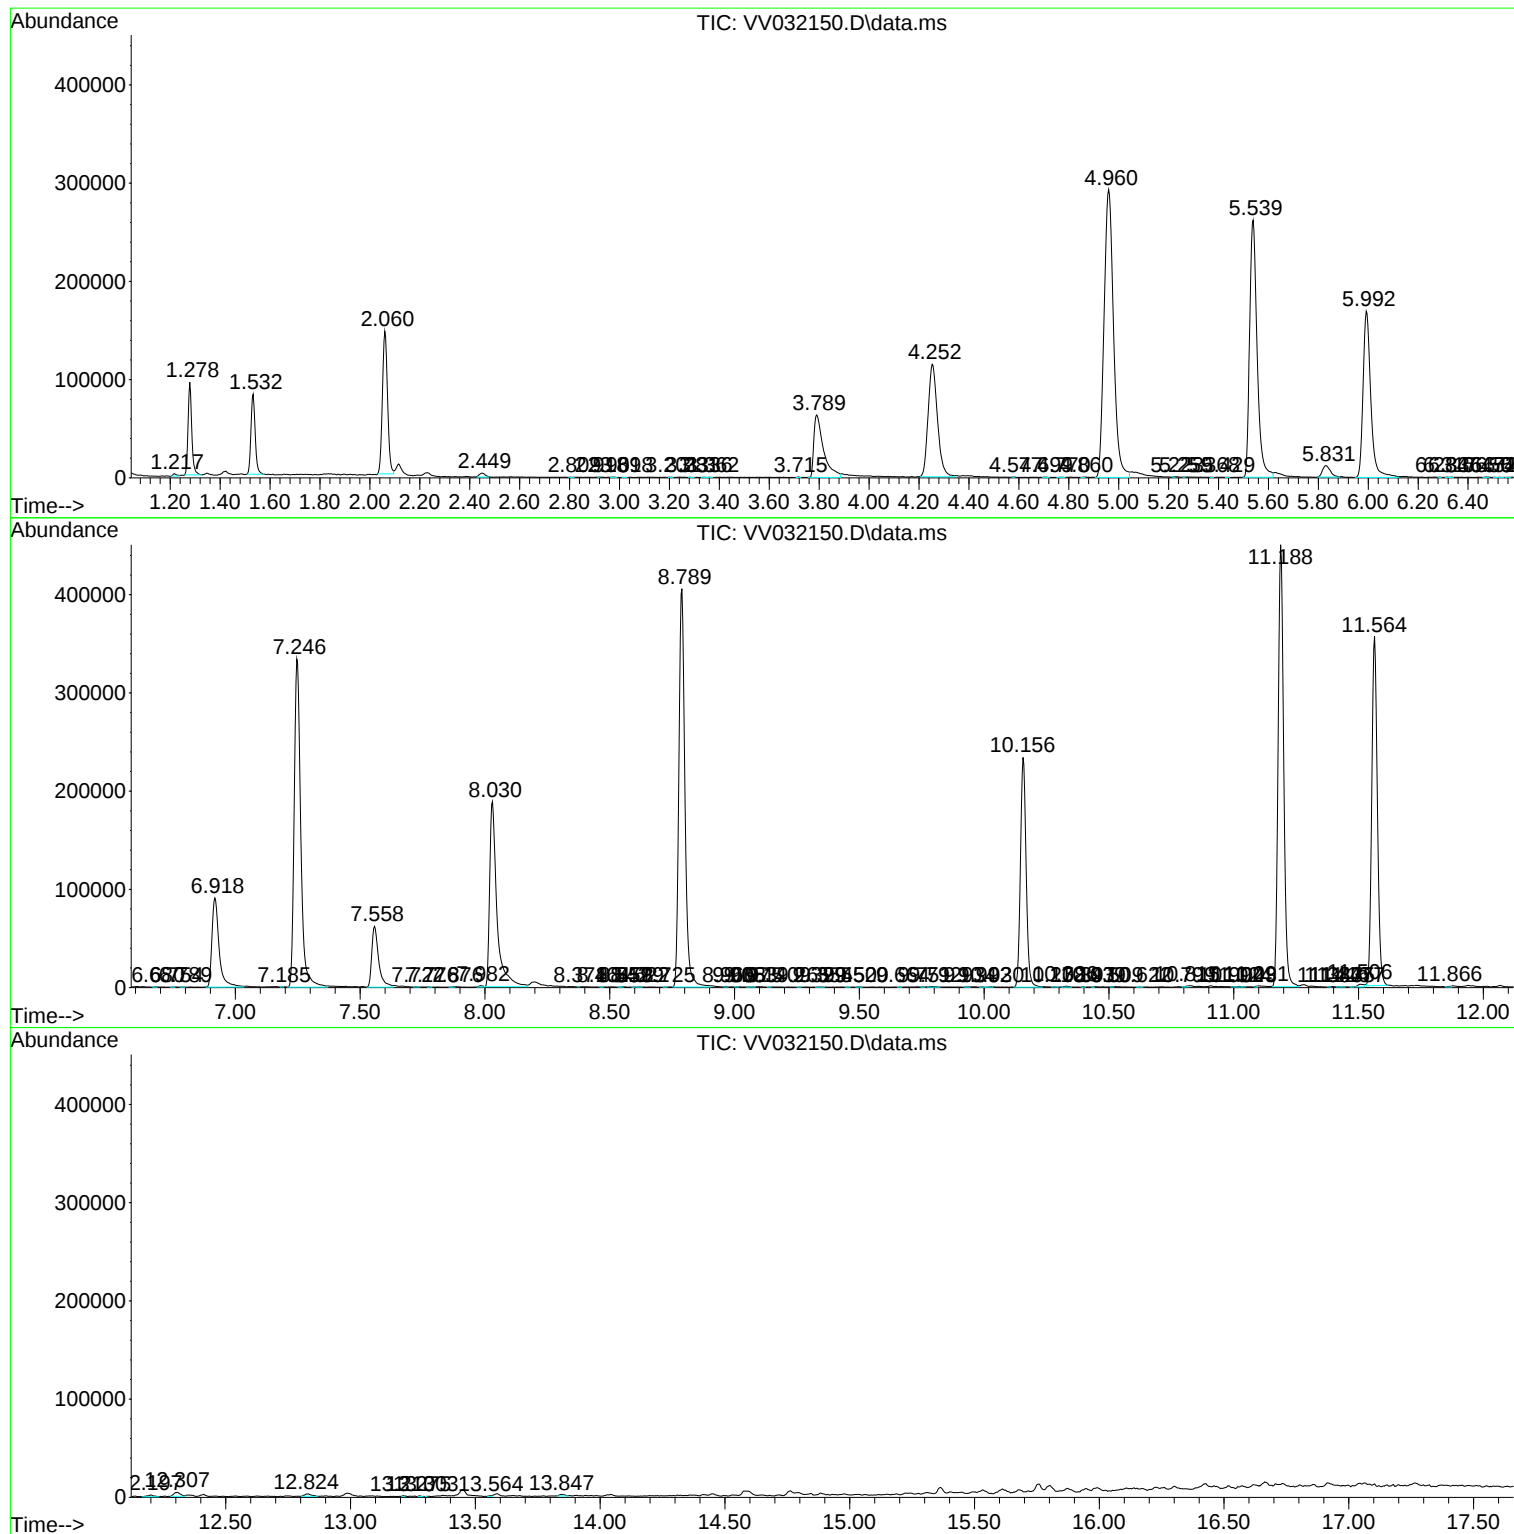

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
Data File : VV032150.D
Acq On : 20 Sep 2023 16:19
Operator : SY/MD
Sample : 04386-22
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK003

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
Data File : VV032150.D
Acq On : 20 Sep 2023 16:19
Operator : SY/MD
Sample : 04386-22
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK003

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc