

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
 Data File : VV032151.D
 Acq On : 20 Sep 2023 17:05
 Operator : SY/MD
 Sample : 04385-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M

Title : VOC Analysis

Signal : TIC: VV032151.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	86	rVB	118756	123139	14.40%	1.782%
2	1.532	146	153	169	rVB	100323	115969	13.57%	1.678%
3	2.060	308	317	330	rBV	188787	269691	31.55%	3.902%
4	2.359	406	410	413	rBV3	407	302	0.04%	0.004%
5	2.452	432	439	446	rVB4	1375	1829	0.21%	0.026%
6	2.571	474	476	477	rBV4	278	77	0.01%	0.001%
7	2.690	511	513	518	rVB2	342	261	0.03%	0.004%
8	2.719	518	522	523	rBV	221	110	0.01%	0.002%
9	2.851	562	563	568	rVB2	223	118	0.01%	0.002%
10	2.950	592	594	597	rVB	241	93	0.01%	0.001%
11	2.976	597	602	607	rBV2	379	320	0.04%	0.005%
12	2.995	607	608	609	rBV2	186	60	0.01%	0.001%
13	3.043	621	623	625	rBV2	180	76	0.01%	0.001%
14	3.404	733	735	742	rBV2	93	63	0.01%	0.001%
15	3.439	744	746	750	rVV	127	55	0.01%	0.001%
16	3.487	758	761	764	rBV2	277	160	0.02%	0.002%
17	3.561	782	784	786	rBV	132	55	0.01%	0.001%
18	3.596	792	795	796	rBV2	229	120	0.01%	0.002%
19	3.789	846	855	895	rBV	65354	178386	20.87%	2.581%
20	4.143	963	965	967	rBV	416	205	0.02%	0.003%
21	4.252	984	999	1024	rBV	125798	323588	37.85%	4.682%
22	4.580	1097	1101	1103	rBV2	328	187	0.02%	0.003%
23	4.622	1111	1114	1116	rBV2	195	92	0.01%	0.001%
24	4.674	1126	1130	1135	rBV2	281	271	0.03%	0.004%
25	4.709	1138	1141	1143	rBV2	217	170	0.02%	0.002%
26	4.789	1163	1166	1169	rBV2	187	123	0.01%	0.002%
27	4.805	1169	1171	1173	rBV	177	71	0.01%	0.001%
28	4.838	1179	1181	1186	rVB2	203	90	0.01%	0.001%
29	4.960	1201	1219	1246	rBV2	325653	854855	100.00%	12.369%
30	5.336	1334	1336	1338	rVB	356	136	0.02%	0.002%
31	5.358	1338	1343	1345	rBV2	140	141	0.02%	0.002%
32	5.439	1365	1368	1369	rBV	132	57	0.01%	0.001%
33	5.535	1386	1398	1424	rBV	297151	617123	72.19%	8.929%
34	5.828	1479	1489	1509	rBV2	10337	23095	2.70%	0.334%
35	5.992	1525	1540	1579	rBV	185079	398213	46.58%	5.762%
36	6.259	1621	1623	1625	rBV2	131	73	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
 Data File : VV032151.D
 Acq On : 20 Sep 2023 17:05
 Operator : SY/MD
 Sample : 04385-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	6.323	1640	1643	1650	rBV2	91	111	0.01%	0.002%
38	6.391	1662	1664	1669	rVB	180	77	0.01%	0.001%
39	6.416	1669	1672	1677	rBV2	222	165	0.02%	0.002%
40	6.442	1678	1680	1683	rVB2	232	89	0.01%	0.001%
41	6.471	1687	1689	1693	rVB2	180	105	0.01%	0.002%
42	6.596	1722	1728	1731	rBV3	668	616	0.07%	0.009%
43	6.751	1772	1776	1777	rBV	190	93	0.01%	0.001%
44	6.793	1784	1789	1791	rVB	167	95	0.01%	0.001%
45	6.918	1817	1828	1860	rBV	100064	194634	22.77%	2.816%
46	7.246	1917	1930	1973	rBV	392445	705601	82.54%	10.209%
47	7.558	2017	2027	2054	rBV	66805	123762	14.48%	1.791%
48	7.719	2075	2077	2080	rBV3	302	180	0.02%	0.003%
49	7.809	2102	2105	2107	rBV	183	106	0.01%	0.002%
50	7.879	2123	2127	2131	rBV2	368	334	0.04%	0.005%
51	7.924	2138	2141	2143	rBV	279	136	0.02%	0.002%
52	7.940	2144	2146	2148	rVB2	188	79	0.01%	0.001%
53	7.956	2148	2151	2154	rBV	140	125	0.01%	0.002%
54	8.030	2164	2174	2206	rBV	193336	376175	44.00%	5.443%
55	8.661	2368	2370	2373	rVB2	193	91	0.01%	0.001%
56	8.680	2373	2376	2380	rBV	268	202	0.02%	0.003%
57	8.789	2397	2410	2437	rBV	460673	769598	90.03%	11.135%
58	8.979	2467	2469	2474	rBV2	450	306	0.04%	0.004%
59	9.037	2485	2487	2489	rVB2	216	75	0.01%	0.001%
60	9.050	2489	2491	2492	rBV2	224	94	0.01%	0.001%
61	9.255	2552	2555	2557	rBV	195	100	0.01%	0.001%
62	9.394	2595	2598	2601	rBV2	215	130	0.02%	0.002%
63	9.542	2638	2644	2646	rBV	248	274	0.03%	0.004%
64	9.580	2653	2656	2660	rVB2	172	110	0.01%	0.002%
65	9.612	2660	2666	2668	rBV	129	128	0.01%	0.002%
66	9.689	2688	2690	2692	rBV2	128	50	0.01%	0.001%
67	9.747	2704	2708	2713	rBV2	147	144	0.02%	0.002%
68	9.770	2713	2715	2719	rVB	213	102	0.01%	0.001%
69	9.796	2719	2723	2725	rBV2	123	99	0.01%	0.001%
70	9.870	2743	2746	2749	rBV3	222	139	0.02%	0.002%
71	9.995	2782	2785	2790	rVB	222	155	0.02%	0.002%
72	10.034	2790	2797	2798	rBV4	752	775	0.09%	0.011%
73	10.095	2812	2816	2818	rBV2	132	114	0.01%	0.002%
74	10.156	2824	2835	2858	rBV	244397	389081	45.51%	5.629%
75	10.275	2870	2872	2877	rVB2	384	271	0.03%	0.004%
76	10.304	2877	2881	2885	rVB3	192	163	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
 Data File : VV032151.D
 Acq On : 20 Sep 2023 17:05
 Operator : SY/MD
 Sample : 04385-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	10.326	2885	2888	2889	rBV	142	88	0.01%	0.001%
78	10.416	2914	2916	2919	rVB2	290	100	0.01%	0.001%
79	10.435	2919	2922	2927	rBV	162	143	0.02%	0.002%
80	10.570	2961	2964	2968	rBV2	191	152	0.02%	0.002%
81	10.644	2984	2987	2990	rBV	154	84	0.01%	0.001%
82	10.908	3067	3069	3072	rBV	147	74	0.01%	0.001%
83	10.995	3095	3096	3099	rVB2	191	53	0.01%	0.001%
84	11.072	3119	3120	3122	rVB2	152	57	0.01%	0.001%
85	11.088	3122	3125	3127	rBV2	171	106	0.01%	0.002%
86	11.188	3145	3156	3181	rBV	515086	804671	94.13%	11.643%
87	11.564	3261	3273	3294	rBV	401361	629141	73.60%	9.103%
88	11.770	3335	3337	3340	rVB	361	175	0.02%	0.003%
89	11.786	3340	3342	3345	rBV	173	113	0.01%	0.002%
90	12.069	3423	3430	3433	rBV2	304	328	0.04%	0.005%
91	12.355	3517	3519	3521	rVB2	188	58	0.01%	0.001%
92	12.699	3623	3626	3630	rVB	209	131	0.02%	0.002%
93	12.725	3630	3634	3636	rBV	401	200	0.02%	0.003%
94	13.085	3744	3746	3748	rBV2	275	147	0.02%	0.002%
95	13.345	3823	3827	3833	rBV3	304	328	0.04%	0.005%
96	13.377	3835	3837	3839	rVB	335	142	0.02%	0.002%
97	13.448	3857	3859	3860	rBV	453	192	0.02%	0.003%
98	13.564	3893	3895	3896	rBV	201	80	0.01%	0.001%
99	13.577	3896	3899	3900	rBV2	277	157	0.02%	0.002%
100	13.840	3979	3981	3993	rVB4	629	715	0.08%	0.010%




Sum of corrected areas: 6911493

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
Data File : VV032151.D
Acq On : 20 Sep 2023 17:05
Operator : SY/MD
Sample : 04385-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

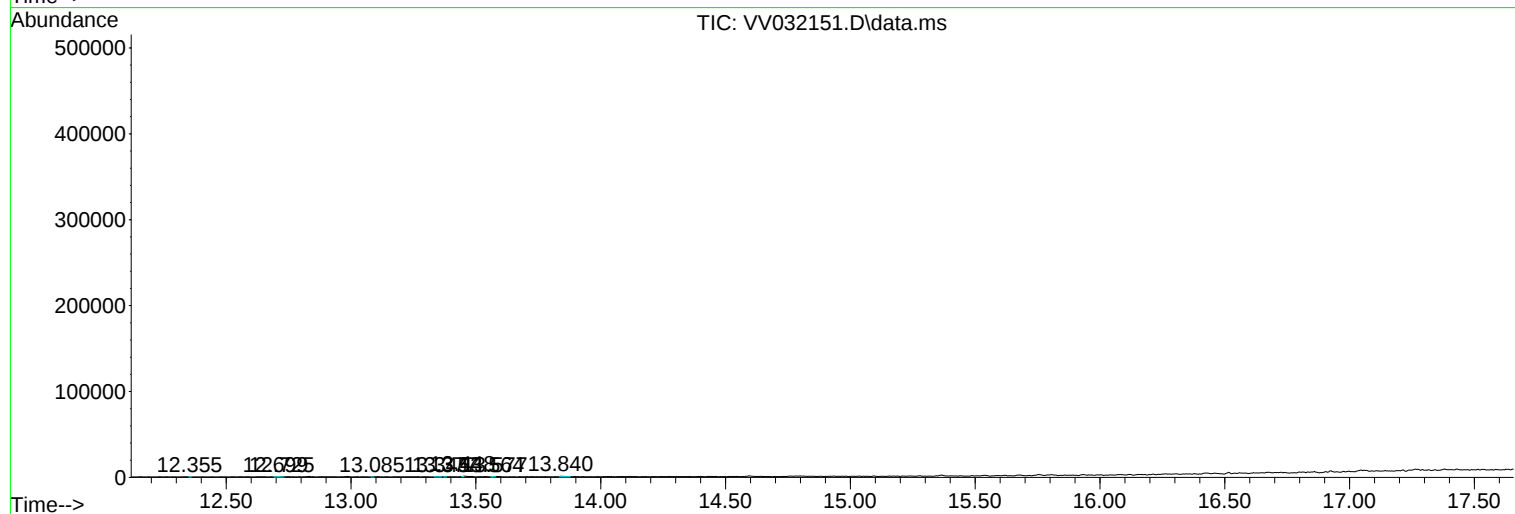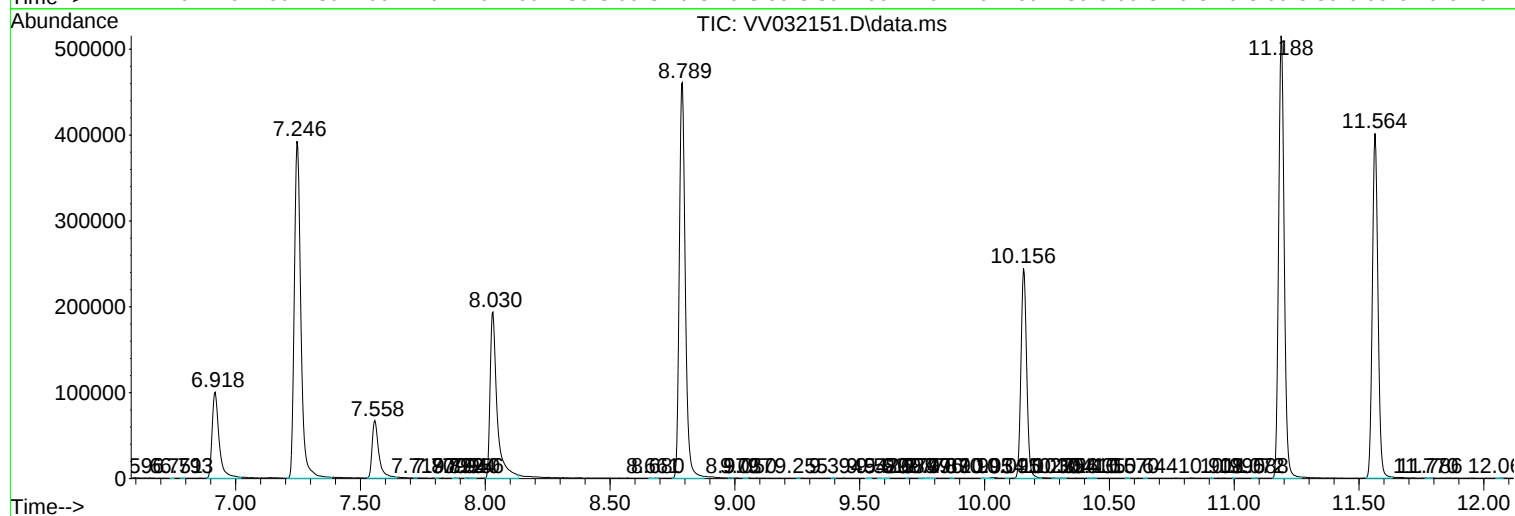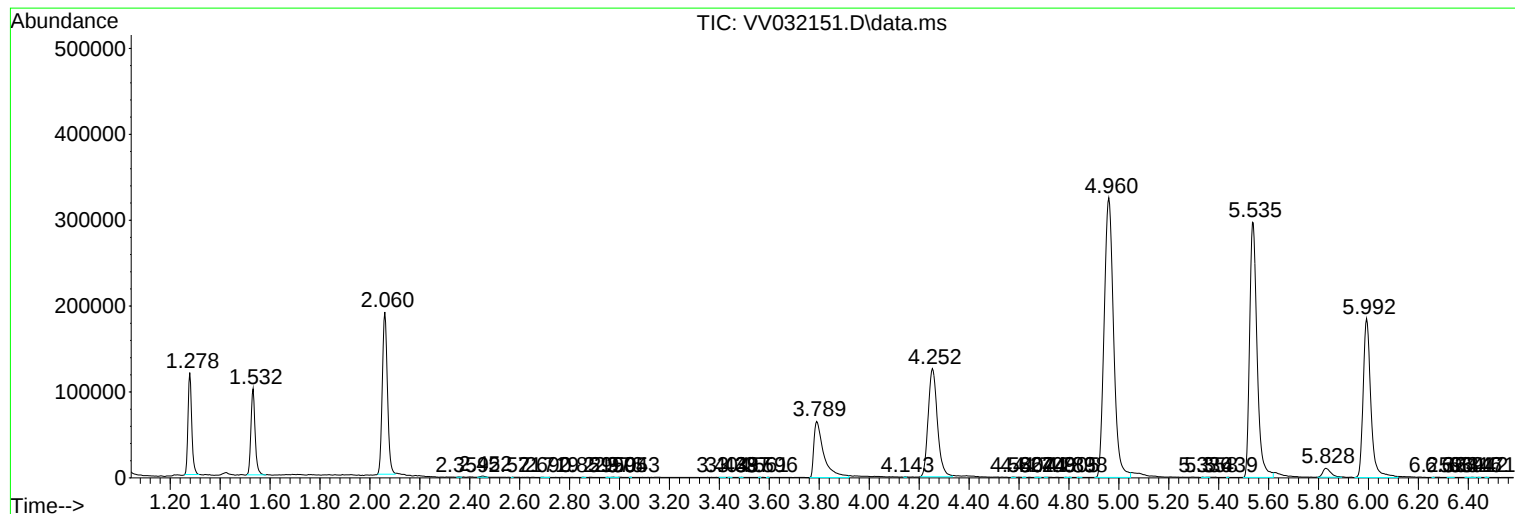

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
Data File : VV032151.D
Acq On : 20 Sep 2023 17:05
Operator : SY/MD
Sample : 04385-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
Data File : VV032151.D
Acq On : 20 Sep 2023 17:05
Operator : SY/MD
Sample : 04385-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------