
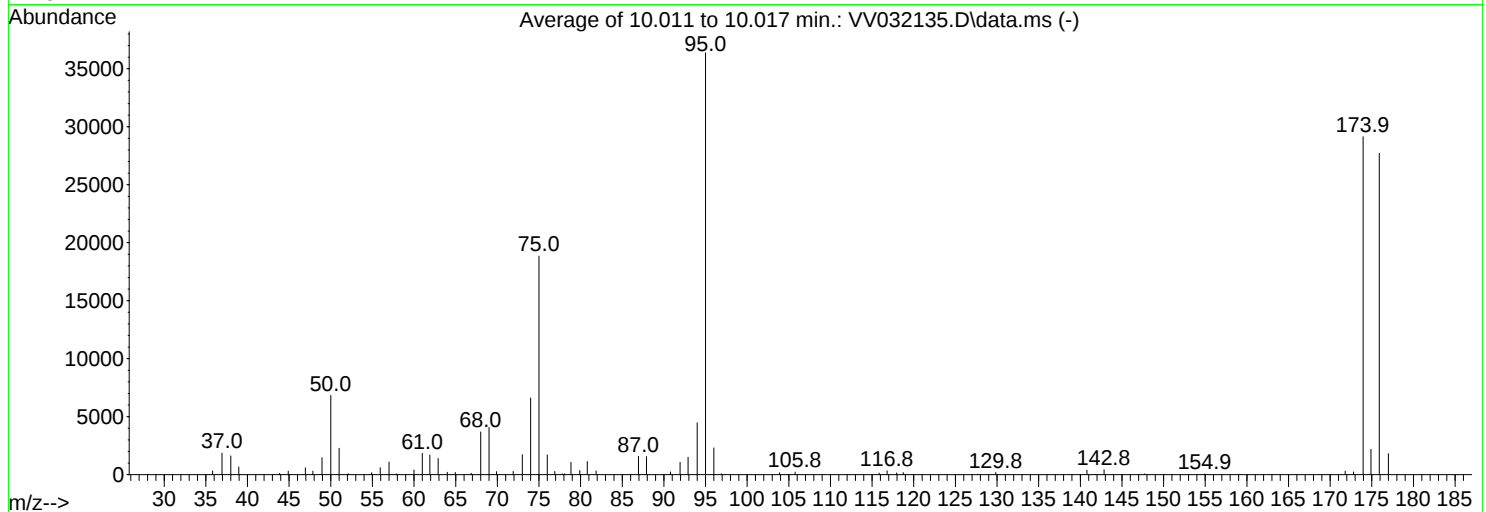


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092023\
Data File : VV032135.D
Acq On : 20 Sep 2023 08:38
Operator : SY/MD
Sample : BFB214
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB214

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Title : VOC Analysis
Last Update : Thu Sep 21 01:37:00 2023

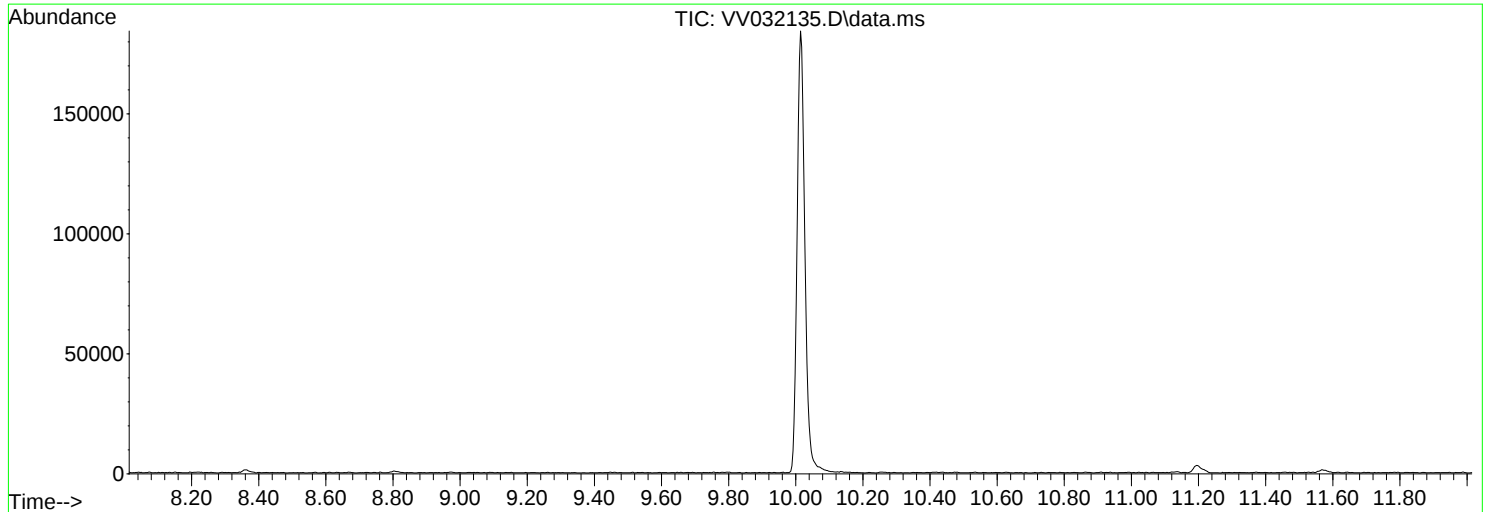

AutoFind: Scans 2790, 2791, 2792; Background Corrected with Scan 2779

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.8	6824	PASS
75	95	30	80	51.8	18851	PASS
95	95	100	100	100.0	36371	PASS
96	95	5	9	6.3	2298	PASS
173	174	0.00	2	0.8	233	PASS
174	95	50	120	80.1	29136	PASS
175	174	5	9	7.5	2176	PASS
176	174	95	105	95.1	27704	PASS
177	176	5	10	6.5	1807	PASS

m/z	Abundance
40.00	183.0
43.90	382.0

Instrument :
MSVOA_V
ClientSampleId :
BFB214

m/z	Abundance
35.80	333.0
36.90	1718.0
38.00	1584.0
39.00	671.0
39.80	181.0
43.80	499.0
44.90	315.0
47.00	601.0
47.80	281.0
48.90	1386.0
50.00	6732.0
51.00	2290.0
52.10	142.0
54.90	159.0
55.90	631.0
57.00	1058.0
60.00	407.0
61.00	1799.0
61.90	1660.0
62.90	1411.0
64.00	178.0
64.90	208.0
66.80	104.0
68.00	3610.0
69.00	3950.0
69.90	301.0
71.90	276.0
73.00	1724.0
74.00	6585.0
75.00	18352.0
76.00	1719.0
76.90	232.0
77.80	202.0
78.80	1057.0
79.90	370.0
80.80	1150.0
81.80	304.0
86.90	1567.0
87.90	1601.0
90.80	220.0
91.90	1047.0
92.90	1560.0
94.00	4268.0
95.00	35144.0
96.00	2255.0
96.90	109.0
103.90	188.0
104.90	100.0
105.70	231.0
115.90	162.0
116.80	326.0
117.90	144.0
118.80	157.0
127.70	110.0
129.90	177.0
140.80	385.0
142.80	393.0
147.70	113.0
155.00	109.0
171.80	247.0
174.00	27624.0
174.90	2031.0
175.90	25984.0
177.00	1786.0

Instrument :
MSVOA_V
ClientSampleId :
BFB214

m/z	Abundance
35.80	322.0
37.00	1896.0
38.00	1674.0
39.00	670.0
39.80	162.0
43.90	490.0
44.90	309.0
46.90	608.0
47.80	326.0
49.00	1533.0
50.00	7075.0
51.00	2364.0
52.10	119.0
54.90	176.0
55.90	620.0
57.00	1125.0
57.90	111.0
60.00	434.0
61.00	1870.0
61.90	1755.0
62.90	1428.0
64.00	212.0
64.90	201.0
66.90	136.0
68.00	3794.0
69.00	4262.0
69.90	280.0
71.90	295.0
73.00	1765.0
74.00	6869.0
75.00	19472.0
76.00	1744.0
76.90	275.0
78.10	211.0
78.80	1090.0
79.90	372.0
80.80	1162.0
81.90	336.0
87.00	1580.0
87.90	1612.0
90.80	236.0
91.90	1102.0
92.90	1521.0
94.00	4605.0
95.00	37616.0
96.00	2368.0
96.90	117.0
103.90	173.0
105.80	235.0
115.90	139.0
116.80	347.0
118.00	163.0
118.70	194.0
129.90	188.0
140.80	401.0
141.80	102.0
142.80	425.0
147.70	108.0
154.90	100.0
171.80	324.0
172.80	362.0
173.90	30192.0
174.90	2252.0
175.90	28680.0
177.00	1862.0

Instrument :
MSVOA_V
ClientSampleId :
BFB214

m/z	Abundance
35.00	289.0
37.00	1918.0
38.00	1589.0
38.90	653.0
39.90	139.0
43.90	504.0
44.90	302.0
46.90	566.0
47.90	309.0
49.00	1457.0
50.00	6665.0
51.00	2190.0
54.90	170.0
56.00	544.0
57.00	1088.0
57.90	114.0
60.00	381.0
61.00	1823.0
61.90	1697.0
62.90	1365.0
64.00	225.0
65.00	184.0
66.90	143.0
68.00	3660.0
69.00	3998.0
69.90	227.0
71.90	276.0
73.00	1682.0
74.00	6384.0
75.00	18728.0
76.00	1612.0
76.90	313.0
78.90	1039.0
79.90	325.0
80.80	1087.0
81.90	321.0
87.00	1565.0
87.90	1463.0
90.80	236.0
92.00	1034.0
92.90	1452.0
94.00	4558.0
95.00	36352.0
96.00	2271.0
103.90	142.0
105.80	215.0
115.80	133.0
116.80	304.0
118.00	165.0
118.70	207.0
129.80	184.0
140.80	394.0
142.90	457.0
171.80	349.0
172.80	337.0
173.90	29592.0
174.90	2244.0
175.90	28448.0
177.00	1773.0

Instrument :
MSVOA_V
ClientSampleId :
BFB214