

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092118\
 Data File : VV007690.D
 Acq On : 21 Sep 2018 11:20
 Operator : SY/MD
 Sample : J4990-14
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0T16

Quant Time: Sep 22 00:03:47 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091918WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Sep 21 03:27:29 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	102091	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	94854	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	49670	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	18291	4.36	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	87.20%
7) Chloroethane-d5	1.59	69	20115	5.10	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	102.00%
11) 1,1-Dichloroethene-d2	2.14	63	35044	3.15	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.00%
20) 2-Butanone-d5	3.96	46	53407	49.89	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	99.78%
24) Chloroform-d	4.41	84	47211	4.72	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.40%
26) 1,2-Dichloroethane-d4	5.09	65	25139	5.08	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.60%
32) Benzene-d6	5.10	84	91125	4.85	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.00%
36) 1,2-Dichloropropane-d6	6.12	67	27149	4.89	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.80%
41) Toluene-d8	7.36	98	90108	4.65	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.00%
43) trans-1,3-Dichloropropene-	7.67	79	9321	4.18	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.60%
46) 2-Hexanone-d5	8.14	63	38838	44.68	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	89.36%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	21887	4.76	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.20%
64) 1,2-Dichlorobenzene-d4	11.68	152	40200	4.90	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.00%


Target Compounds					Ovalue
13) Acetone	2.21	43	21805	21.146 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV092118\
Data File : VV007690.D
Acq On : 21 Sep 2018 11:20
Operator : SY/MD
Sample : J4990-14
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0T16

Quant Time: Sep 22 00:03:47 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091918WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Sep 21 03:27:29 2018
Response via : Initial Calibration

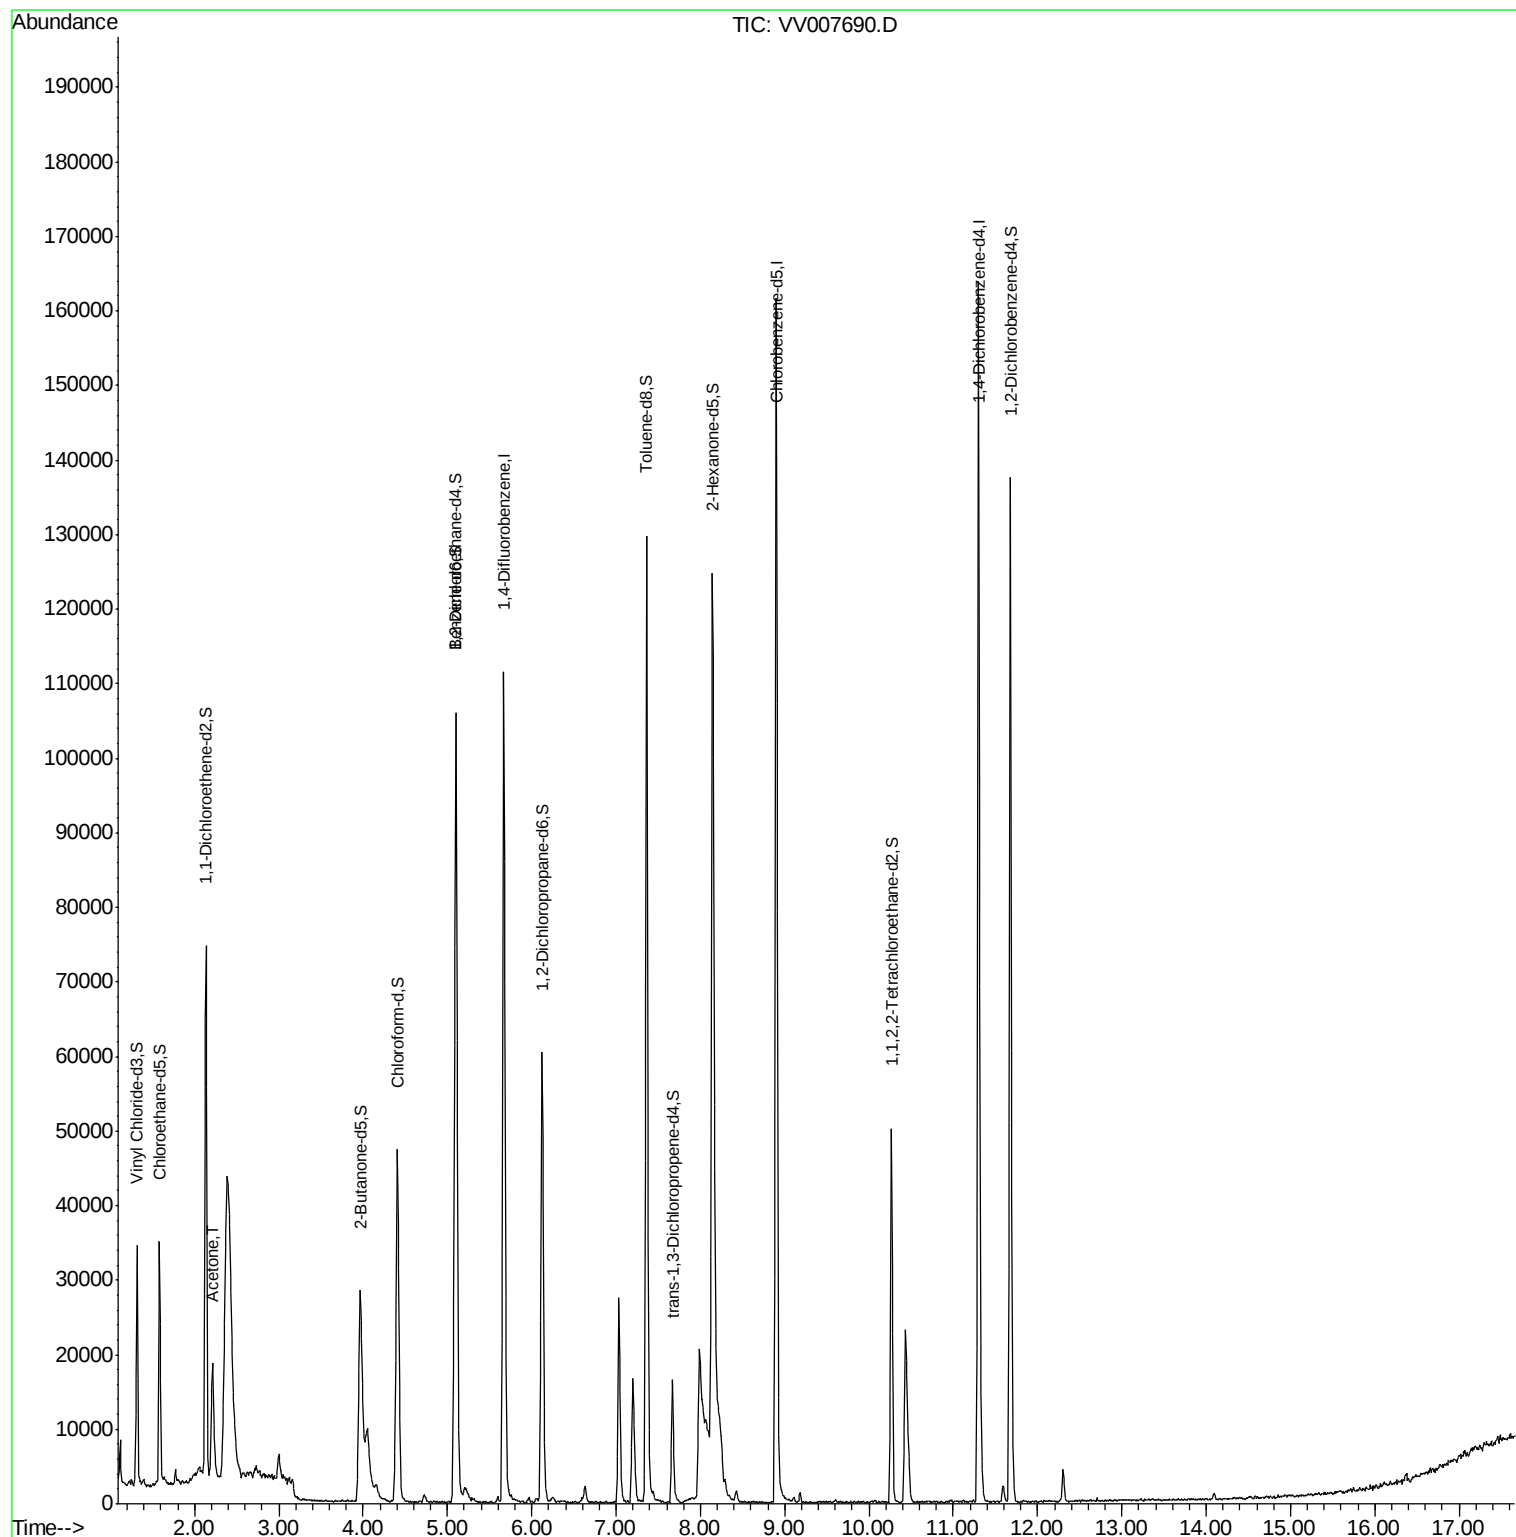

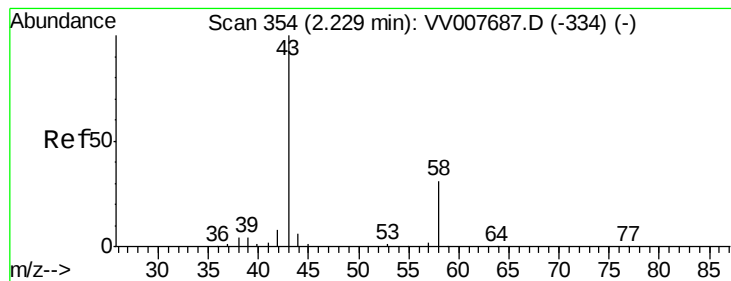

#13

Acetone

Concen: 21.146 ug/L

RT: 2.21 min Scan# 349

Delta R.T. -0.00 min

Lab File: VV007690.D

Acq: 21 Sep 2018 11:20

Instrument :
MSVOA_V
ClientSampleId :
COT16

Tot Ion: 43 Resp: 21805

Ion Ratio Lower Upper

43 100

58 34.5 0.0 63.6

