

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092118\
 Data File : VV007697.D
 Acq On : 21 Sep 2018 14:33
 Operator : SY/MD
 Sample : J4990-19
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0T21

Quant Time: Sep 22 00:19:38 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091918WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Sep 21 03:27:29 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	98900	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	90800	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	47978	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	16336	4.02	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	80.40%
7) Chloroethane-d5	1.59	69	18661	4.89	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.80%
11) 1,1-Dichloroethene-d2	2.13	63	31233	2.90	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	58.00%#
20) 2-Butanone-d5	3.96	46	53597	51.69	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	103.38%
24) Chloroform-d	4.41	84	44554	4.59	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.80%
26) 1,2-Dichloroethane-d4	5.09	65	24130	5.04	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.80%
32) Benzene-d6	5.10	84	82813	4.60	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.00%
36) 1,2-Dichloropropane-d6	6.12	67	25492	4.80	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.00%
41) Toluene-d8	7.36	98	81651	4.40	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.00%
43) trans-1,3-Dichloropropene-	7.67	79	8522	3.99	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	79.80%
46) 2-Hexanone-d5	8.14	63	37628	45.22	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	90.44%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	21268	4.83	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.60%
64) 1,2-Dichlorobenzene-d4	11.68	152	38861	4.91	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.20%


Target Compounds				Ovalue
13) Acetone	2.21	43	12831	12.845 ug/L 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV092118\
Data File : VV007697.D
Acq On : 21 Sep 2018 14:33
Operator : SY/MD
Sample : J4990-19
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0T21

Quant Time: Sep 22 00:19:38 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091918WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Sep 21 03:27:29 2018
Response via : Initial Calibration

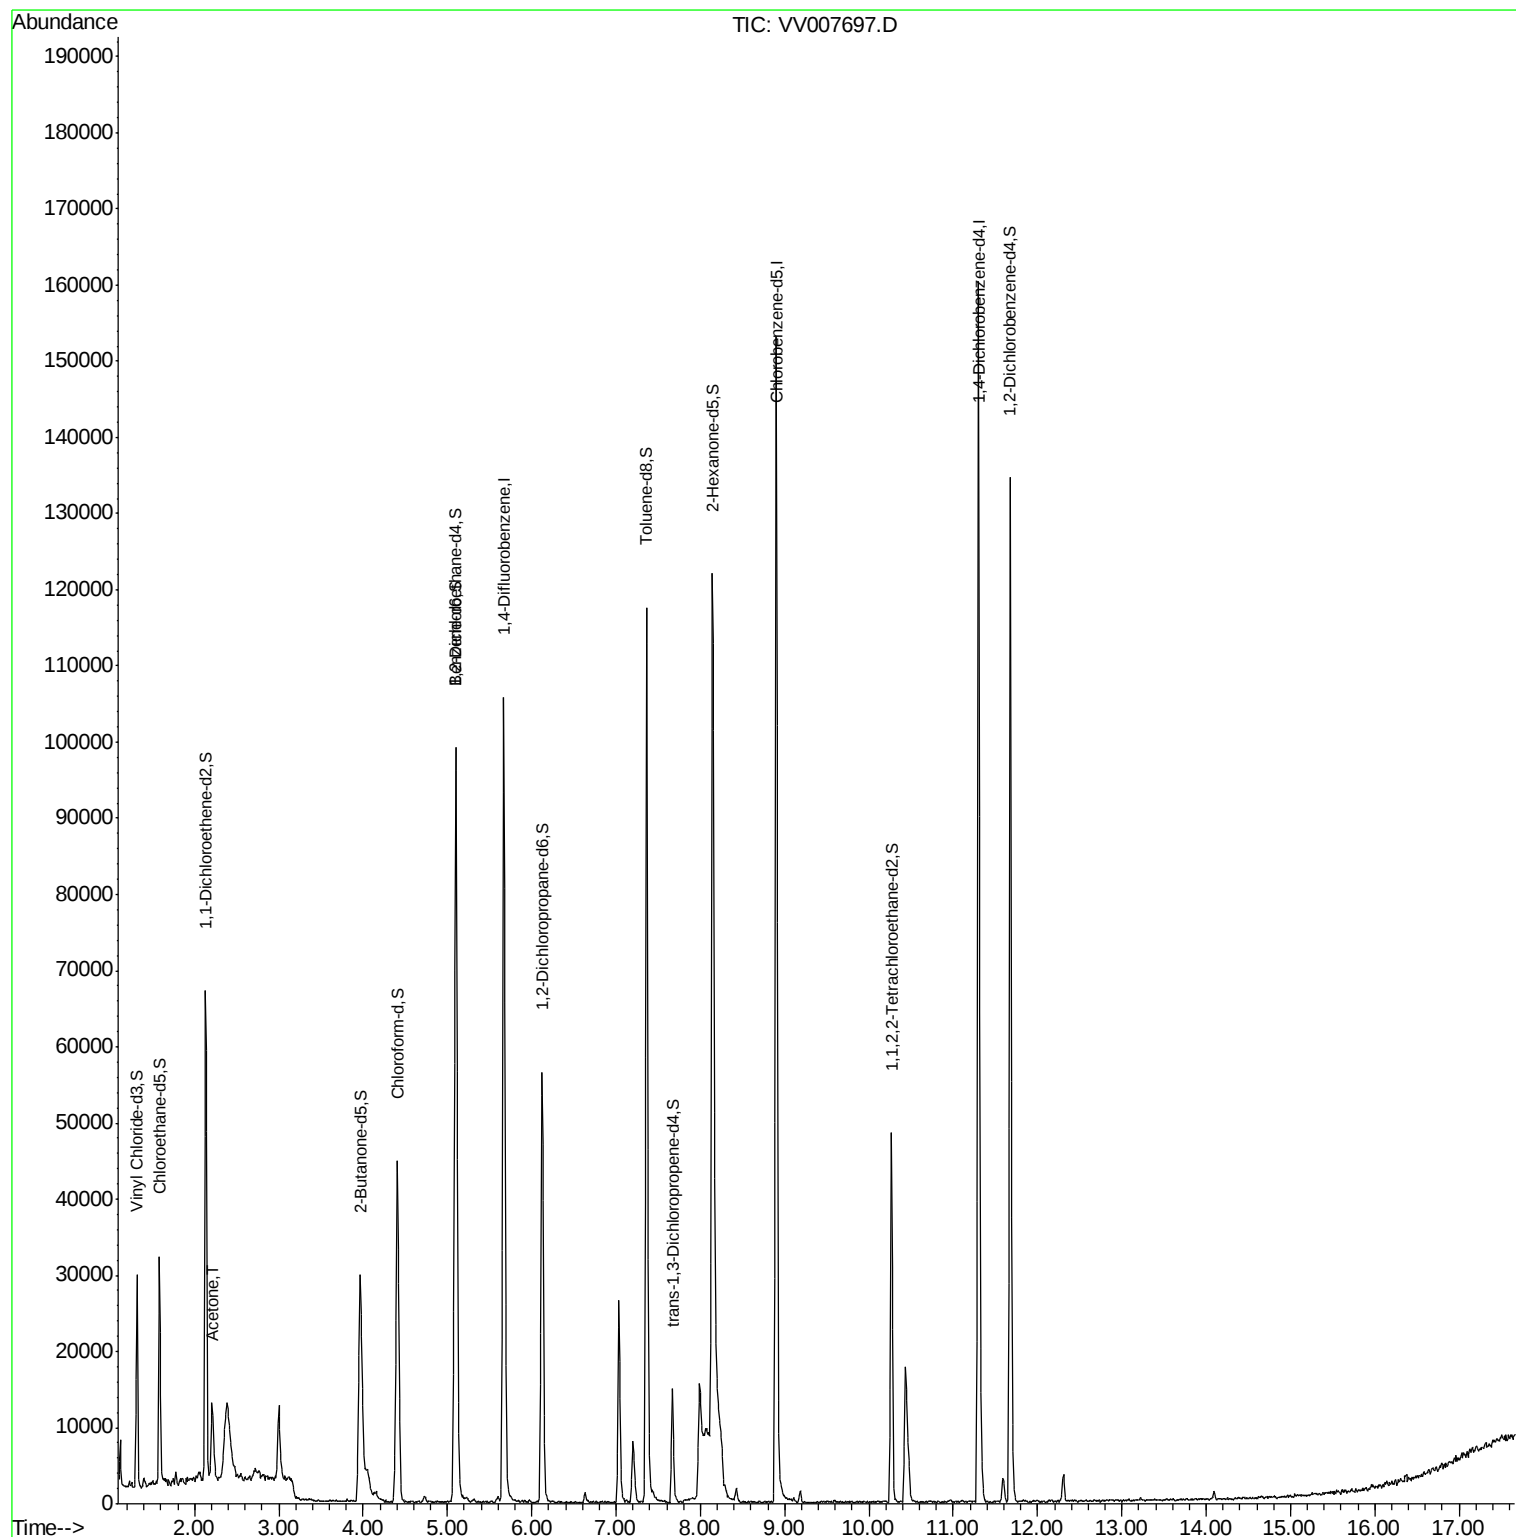

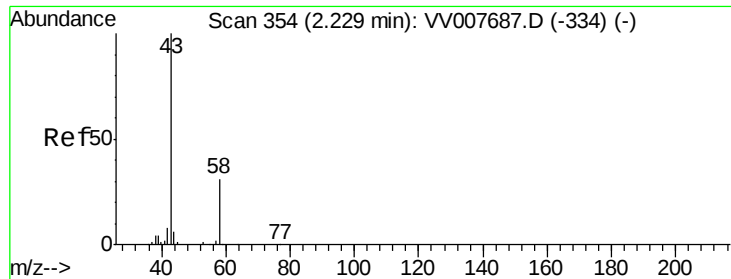

#13

Acetone

Concen: 12.845 ug/L

RT: 2.21 min Scan# 348

Delta R.T. -0.01 min

Lab File: VV007697.D

Acq: 21 Sep 2018 14:33

Instrument :

MSVOA_V

ClientSampleId :

C0T21

Tot Ion: 43 Resp: 12831

Ion Ratio Lower Upper

43 100

58 32.6 0.0 63.6

