

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092118\
 Data File : VV007693.D
 Acq On : 21 Sep 2018 12:42
 Operator : SY/MD
 Sample : J4990-15
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0T17

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.1

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091918WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.116	3	8	14	rVB2	5795	4995	1.58%	0.192%
2	1.319	61	71	81	rVV	30347	34167	10.82%	1.311%
3	1.585	147	154	165	rBV	29194	33973	10.76%	1.304%
4	1.772	205	212	219	rVB	6863	8432	2.67%	0.324%
5	2.135	315	325	336	rBV	65580	91913	29.12%	3.527%
6	2.212	337	349	362	rVV2	13566	28626	9.07%	1.099%
7	2.389	378	404	437	rBV2	17072	87826	27.82%	3.370%
8	3.000	587	594	603	rVB7	1742	3302	1.05%	0.127%
9	3.965	879	894	915	rBV	30964	94089	29.81%	3.611%
10	4.405	1014	1031	1051	rBV	46553	110277	34.94%	4.232%
11	5.100	1231	1247	1274	rBV2	102280	241815	76.61%	9.280%
12	5.669	1410	1424	1445	rBV	105389	207547	65.75%	7.965%
13	6.126	1549	1566	1590	rBV	58201	118639	37.59%	4.553%
14	7.035	1838	1849	1866	rBV2	28056	50399	15.97%	1.934%
15	7.203	1887	1901	1915	rBV5	5024	11511	3.65%	0.442%
16	7.363	1937	1951	1966	rBV	121789	210365	66.65%	8.073%
17	7.669	2035	2046	2066	rBV	16382	27785	8.80%	1.066%
18	7.990	2131	2146	2150	rBV3	15749	27680	8.77%	1.062%
19	8.145	2183	2194	2236	rVB3	128057	315647	100.00%	12.113%
20	8.421	2273	2280	2290	rBV6	1757	3201	1.01%	0.123%
21	8.900	2417	2429	2453	rBV	152207	252738	80.07%	9.699%
22	10.267	2843	2854	2871	rBV2	48599	77641	24.60%	2.979%
23	10.434	2894	2906	2928	rBV	20041	51344	16.27%	1.970%
24	11.299	3164	3175	3199	rBV	161197	269192	85.28%	10.330%
25	11.592	3255	3266	3276	rBV4	4441	7632	2.42%	0.293%
26	11.675	3281	3292	3311	rBV	137412	227966	72.22%	8.748%
27	12.302	3475	3487	3498	rVB3	4332	7143	2.26%	0.274%


Sum of corrected areas: 2605845

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV092118\
Data File : VV007693.D
Acq On : 21 Sep 2018 12:42
Operator : SY/MD
Sample : J4990-15
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0T17

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091918WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

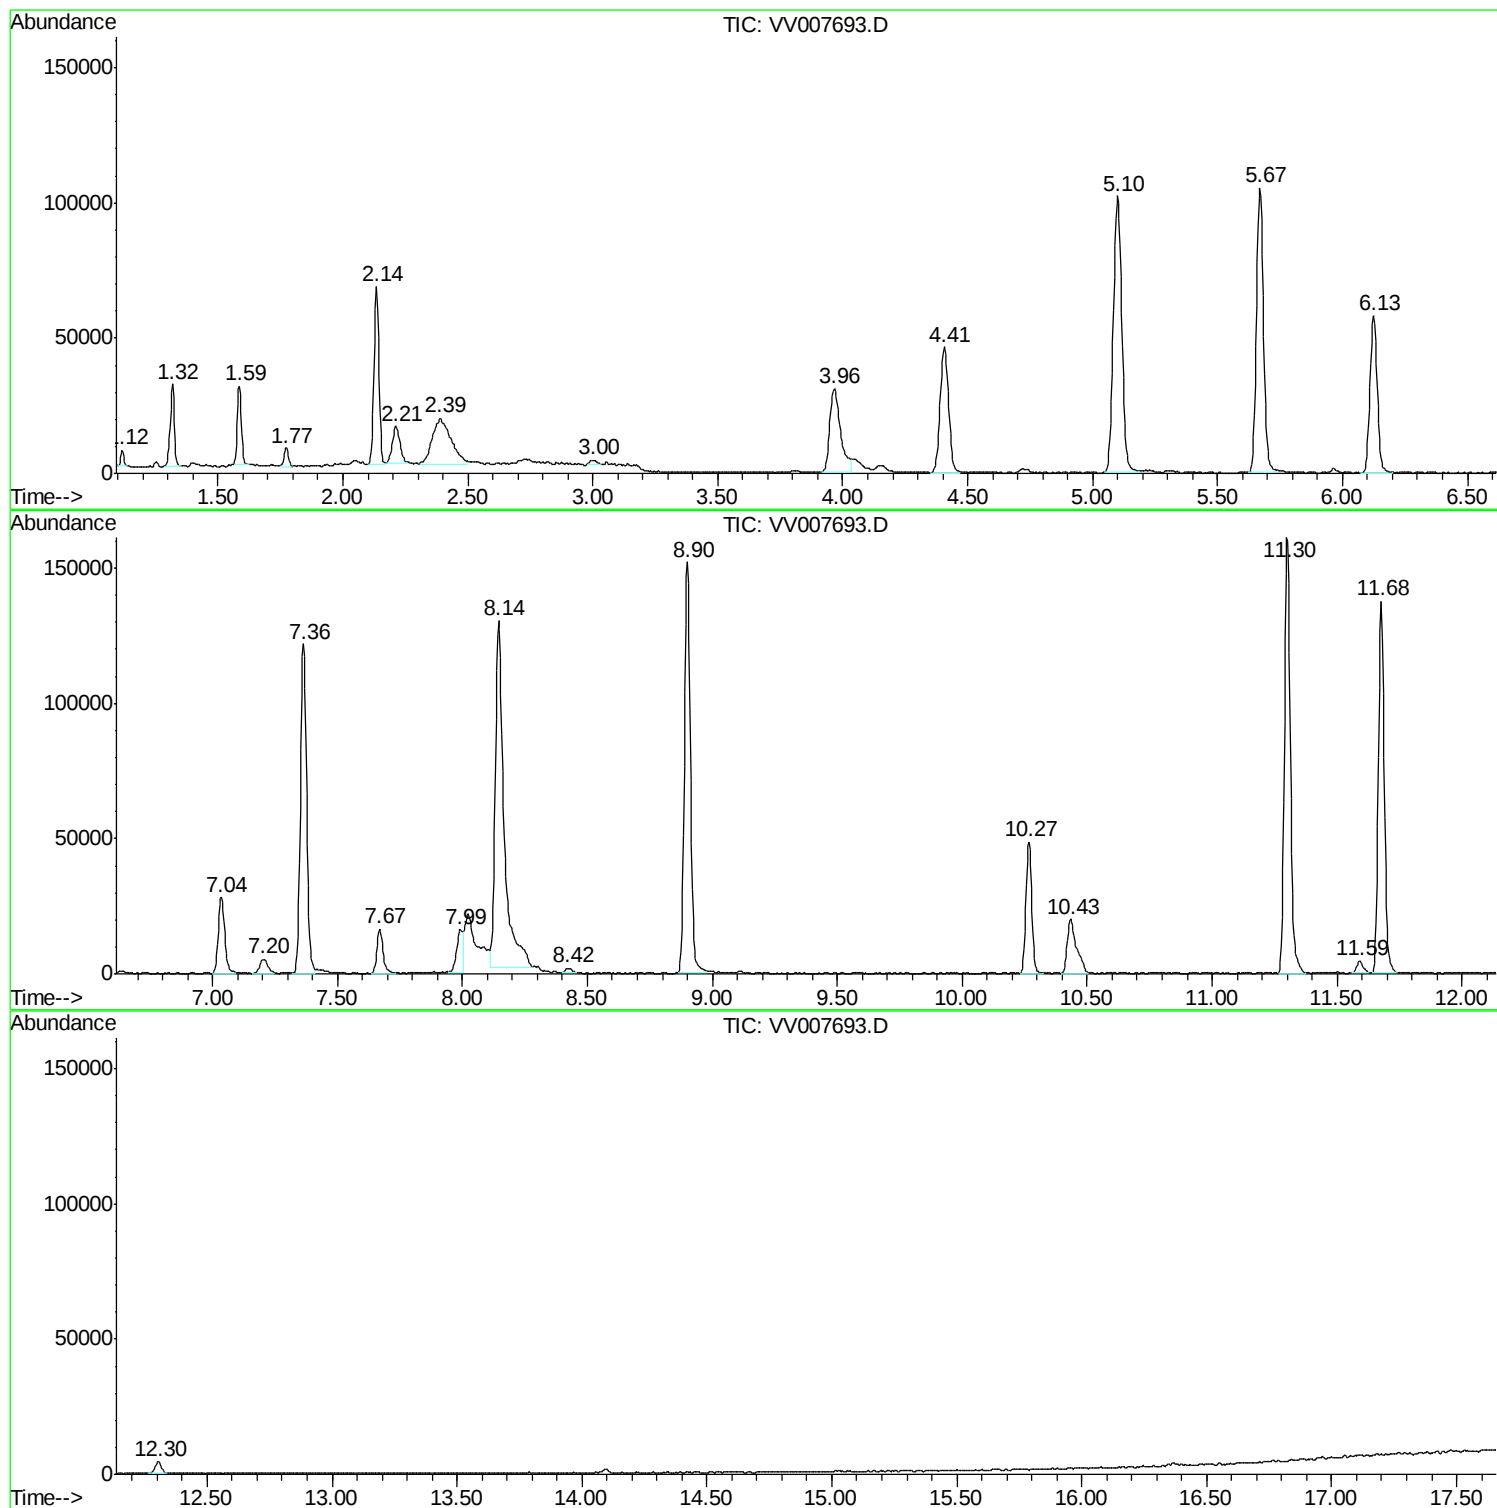

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV092118\
Data File : VV007693.D
Acq On : 21 Sep 2018 12:42
Operator : SY/MD
Sample : J4990-15
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0T17










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091918WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.39	2.12 ug/L	87826	1,4-Difluorobenzene	5.67

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Isopropyl Alcohol	60	C3H8O	000067-63-0	80
2		Isopropyl Alcohol	60	C3H8O	000067-63-0	72
3		Isopropyl Alcohol	60	C3H8O	000067-63-0	72
4		Hydrazine, ethyl-	60	C2H8N2	000624-80-6	40
5		Propane, 2-ethoxy-	88	C5H12O	000625-54-7	40

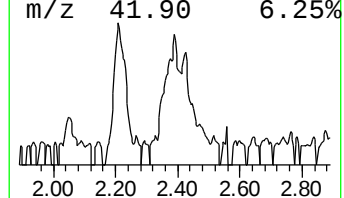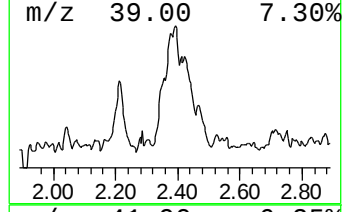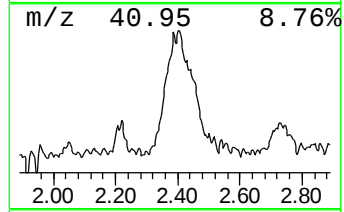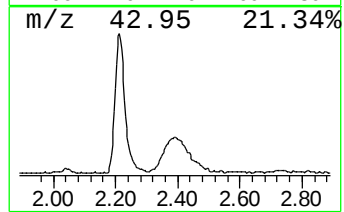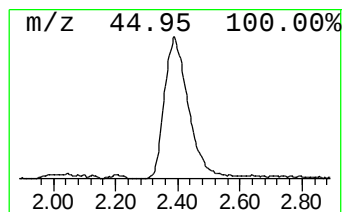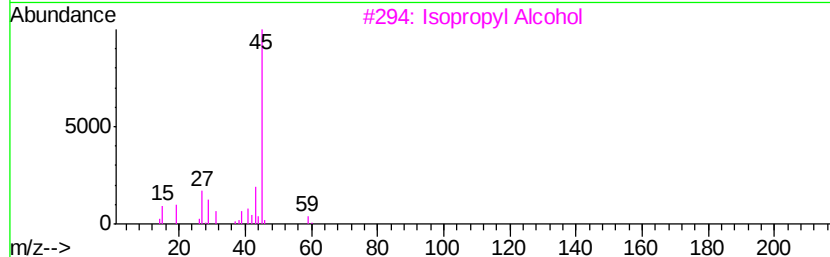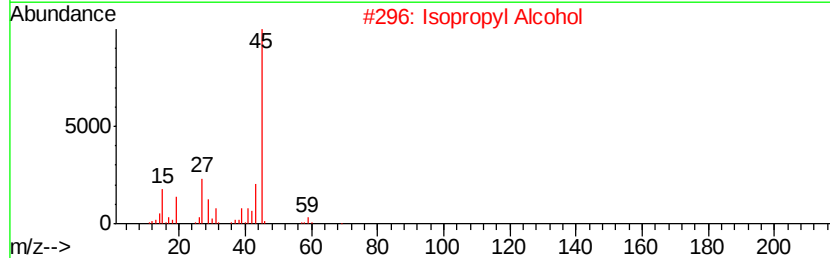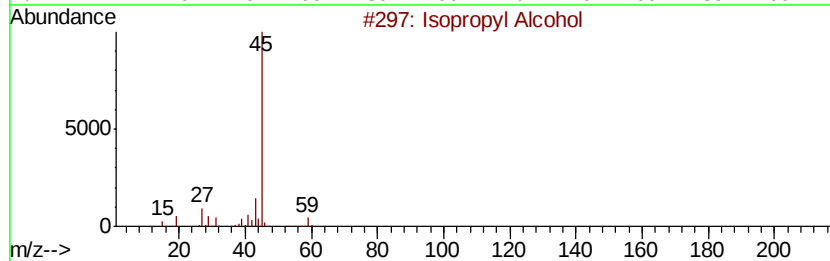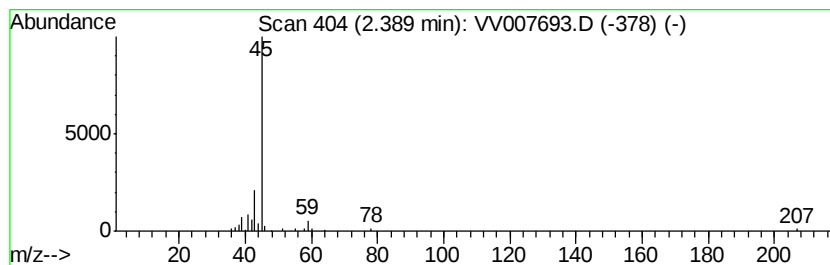

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV092118\
Data File : VV007693.D
Acq On : 21 Sep 2018 12:42
Operator : SY/MD
Sample : J4990-15
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0T17

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091918WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.39	2.1	ug/L	87826	1	5.67	207547	5.0