


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092118\
Data File : VV007686.D
Acq On : 21 Sep 2018 08:56
Operator : SY/MD
Sample : BFB62
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB62

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091918WMA.M
Title : TRACE VOA SOM01.0
Last Update : Fri Sep 21 03:27:29 2018

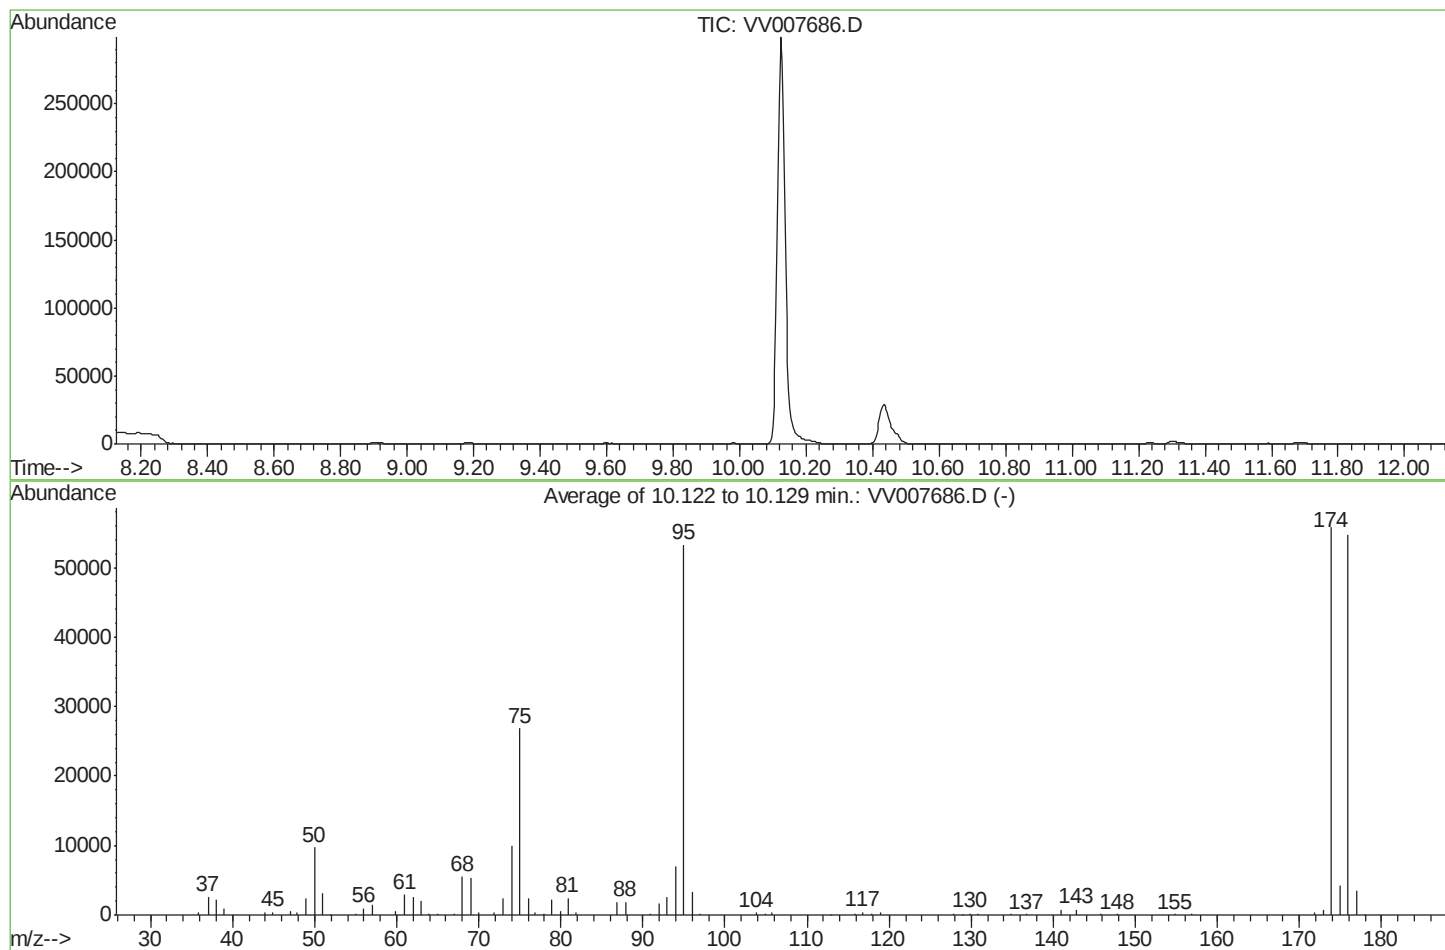

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	9709	PASS
75	95	30	80	50.4	26880	PASS
95	95	100	100	100.0	53282	PASS
96	95	5	9	6.2	3296	PASS
173	174	0.00	2	1.2	679	PASS
174	95	50	120	104.7	55789	PASS
175	174	5	9	7.5	4157	PASS
176	174	95	101	98.1	54704	PASS
177	176	5	9	6.5	3574	PASS

Scan 2796 (10.080 min): VV007686.D
BFB62

m/z	Abundance
43.90	244.0
206.80	102.0

Instrument :
MSVOA_V
ClientSampleId :
BFB62

m/z	Abundance
35.90	436.0
37.00	2649.0
38.00	2225.0
39.00	974.0
44.00	683.0
44.90	465.0
47.00	560.0
47.90	402.0
49.00	2578.0
50.00	9952.0
51.00	3150.0
51.90	103.0
55.00	183.0
56.00	886.0
57.00	1457.0
59.90	490.0
61.00	2936.0
62.00	2668.0
63.00	2220.0
63.90	216.0
64.90	121.0
67.00	182.0
68.00	5500.0
69.00	5305.0
69.90	458.0
71.90	297.0
73.00	2405.0
74.00	9910.0
75.00	27272.0
76.00	2448.0
76.90	337.0
77.90	237.0
78.90	2282.0
79.90	579.0
80.90	2513.0
81.90	462.0
86.90	1933.0
87.90	1979.0
90.90	279.0
91.90	1749.0
93.00	2721.0
94.00	7015.0
95.00	53648.0
96.00	3449.0
97.00	117.0
103.80	354.0
104.90	183.0
105.80	259.0
115.80	240.0
116.80	433.0
117.90	235.0
118.90	291.0
127.90	236.0
130.00	233.0
130.80	130.0
134.90	149.0
136.80	167.0
140.90	722.0
142.90	793.0
145.80	123.0
147.80	161.0
154.90	172.0
156.90	105.0
171.80	301.0
172.90	732.0
173.90	54832.0
174.90	4177.0
175.90	53192.0
176.90	3613.0
177.90	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB62

m/z	Abundance
35.90	383.0
37.00	2406.0
37.90	2014.0
38.90	902.0
43.90	538.0
44.90	354.0
47.00	568.0
47.90	304.0
49.00	2074.0
50.00	9175.0
51.00	2890.0
55.00	182.0
56.00	951.0
57.00	1442.0
59.90	564.0
61.00	2697.0
62.00	2596.0
63.00	1897.0
64.00	221.0
65.00	137.0
67.00	188.0
68.00	5221.0
69.00	5160.0
70.00	430.0
71.90	275.0
73.00	2235.0
74.00	9633.0
75.00	25720.0
76.00	2285.0
76.90	260.0
77.90	224.0
78.90	2188.0
79.90	607.0
80.90	2231.0
81.80	442.0
86.90	1704.0
87.90	1696.0
90.80	238.0
91.90	1577.0
92.90	2483.0
94.00	6733.0
95.00	51136.0
96.00	3053.0
97.00	129.0
103.90	300.0
104.90	143.0
105.70	304.0
112.80	102.0
115.90	222.0
116.80	456.0
117.90	186.0
118.90	300.0
127.90	180.0
129.00	103.0
129.90	253.0
130.80	114.0
134.90	121.0
136.70	121.0
140.90	678.0
142.80	760.0
145.70	118.0
147.90	167.0
154.80	176.0
156.90	157.0
171.80	328.0
172.90	611.0
173.90	55064.0
174.90	4007.0
175.90	54448.0
176.90	3445.0

Instrument :
MSVOA_V
ClientSampleId :
BFB62

m/z	Abundance
35.90	415.0
37.00	2749.0
38.00	2173.0
38.90	985.0
43.90	620.0
44.90	415.0
47.00	607.0
47.90	372.0
49.00	2454.0
50.00	10002.0
51.00	3170.0
55.00	195.0
56.00	993.0
57.00	1493.0
59.90	560.0
61.00	2985.0
62.00	2762.0
63.00	2134.0
63.90	226.0
65.00	133.0
67.00	197.0
68.00	5666.0
69.00	5356.0
69.90	440.0
71.90	294.0
73.00	2410.0
74.00	10162.0
75.00	27648.0
76.00	2464.0
76.90	301.0
77.90	245.0
78.90	2319.0
79.90	612.0
80.90	2504.0
81.80	476.0
86.90	1898.0
87.90	1917.0
90.90	260.0
91.90	1735.0
92.90	2714.0
94.00	7214.0
95.00	55064.0
96.00	3386.0
97.00	132.0
103.80	356.0
104.80	186.0
105.70	298.0
112.80	103.0
115.90	249.0
116.80	472.0
117.90	221.0
118.90	313.0
127.90	226.0
128.90	102.0
129.90	255.0
130.90	131.0
134.90	147.0
136.70	157.0
140.90	767.0
142.90	814.0
145.80	130.0
147.80	169.0
154.90	179.0
156.90	135.0
171.80	316.0
172.90	694.0
173.90	57472.0
174.90	4289.0
175.90	56472.0
176.90	3666.0

Instrument :
MSVOA_V
ClientSampleId :
BFB62