


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092119\
Data File : VV012922.D
Acq On : 20 Sep 2019 13:41
Operator : SY/MD
Sample : BFB42
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB42

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091719WMA.M
Title : TRACE VOA SOM01.0
Last Update : Mon Sep 23 15:47:50 2019

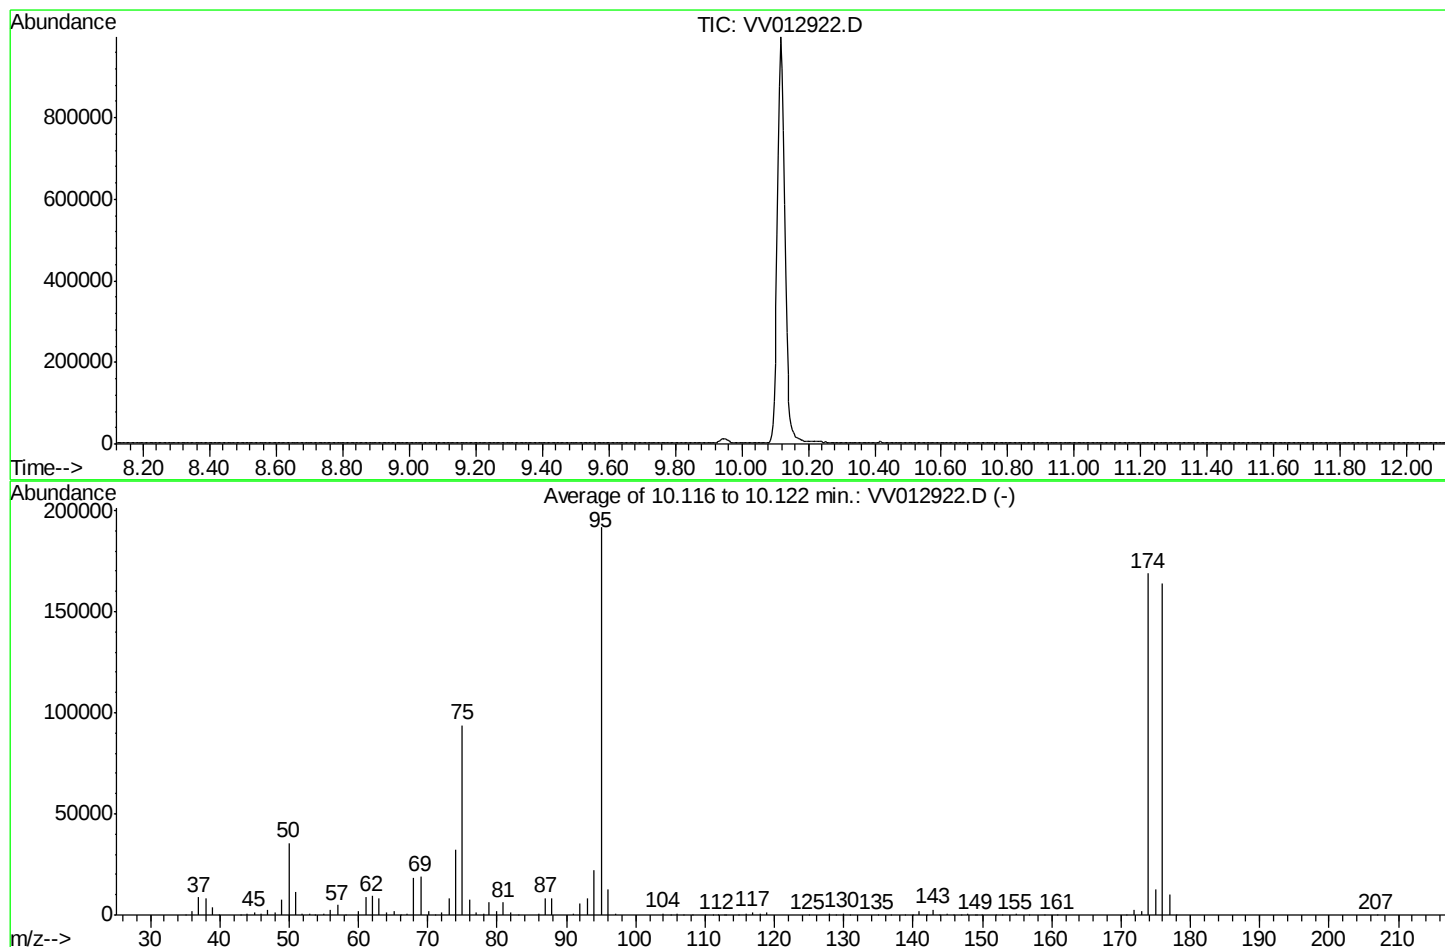

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2793

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	35538	PASS
75	95	30	80	48.9	93738	PASS
95	95	100	100	100.0	191637	PASS
96	95	5	9	6.7	12926	PASS
173	174	0.00	2	1.2	2097	PASS
174	95	50	120	88.1	168832	PASS
175	174	5	9	7.5	12607	PASS
176	174	95	101	97.2	164181	PASS
177	176	5	9	6.1	10007	PASS

m/z	Abundance
35.20	114.0
36.00	1985.0
37.00	9485.0
38.00	8595.0
39.00	3780.0
40.00	1221.0
43.10	127.0
44.00	1917.0
45.00	1563.0
46.00	372.0
47.00	2738.0
48.00	1178.0
49.00	8079.0
50.00	36432.0
51.00	11920.0
52.00	585.0
52.90	310.0
53.70	178.0
55.10	431.0
56.00	2953.0
57.00	4857.0
58.10	206.0
60.00	1779.0
61.00	9372.0
62.00	9629.0
63.00	8021.0
64.00	1330.0
65.10	2009.0
66.00	193.0
66.90	522.0
68.00	18480.0
69.00	19672.0
70.00	1809.0
72.00	1030.0
73.00	8823.0
74.00	32912.0
75.00	96088.0
76.00	7890.0
76.90	1289.0
78.00	893.0
78.90	6174.0
79.90	1806.0
80.90	6526.0
81.90	1398.0
83.20	176.0
85.90	409.0
86.90	8750.0
87.90	8592.0
91.00	764.0
92.00	5974.0
93.00	8258.0
94.00	22488.0
95.00	196352.0
96.00	13890.0
97.10	372.0
104.00	790.0
104.90	282.0
105.90	788.0
107.00	240.0
108.20	111.0
110.00	116.0
111.10	120.0
111.90	204.0
113.00	139.0
114.80	249.0
115.80	852.0
116.90	1410.0
118.00	654.0
118.90	1097.0
127.90	658.0
128.80	305.0
129.90	812.0
131.00	375.0
134.90	320.0
136.90	279.0
139.80	118.0
140.90	1863.0
142.90	2748.0
143.90	187.0
144.90	1061.0
145.90	291.0
146.90	144.0
147.80	536.0
148.90	161.0
149.90	158.0
152.80	133.0
154.80	606.0
156.80	348.0
158.80	302.0
160.80	231.0
170.90	335.0
171.90	2637.0

Instrument :
MSVOA_V
ClientSampleId :
BFB42

173.00	2160.0
173.90	167936.0
174.90	12796.0
175.90	164480.0
177.00	9984.0
178.00	281.0
206.90	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB42

m/z	Abundance
35.10	147.0
36.00	1798.0
37.00	9140.0
38.00	8296.0
39.00	3790.0
40.00	1195.0
43.10	162.0
44.00	1927.0
45.00	1549.0
46.00	378.0
47.00	2849.0
48.00	1086.0
49.00	8070.0
50.00	36624.0
51.00	11984.0
51.90	541.0
52.90	357.0
53.80	121.0
55.10	438.0
56.00	2907.0
57.00	4859.0
58.10	242.0
60.00	1791.0
61.00	9435.0
62.00	9650.0
63.00	8174.0
64.00	1171.0
65.10	1974.0
66.10	185.0
66.90	494.0
68.00	18792.0
69.00	19624.0
70.00	1734.0
71.00	124.0
72.10	1166.0
73.00	8656.0
74.00	33040.0
75.00	96792.0
76.00	8108.0
77.00	1234.0
78.00	930.0
78.90	6259.0
79.90	1709.0
80.90	6468.0
81.90	1509.0
83.10	192.0
86.00	397.0
86.90	8794.0
87.90	8507.0
91.00	728.0
92.00	6146.0
93.00	8411.0
94.00	22952.0
95.00	198208.0
96.00	13284.0
97.10	425.0
104.00	842.0
105.00	271.0
105.90	826.0
106.90	223.0
109.90	145.0
111.10	173.0
111.80	172.0
112.70	122.0
114.80	213.0
115.90	831.0
116.90	1538.0
117.90	678.0
118.90	1043.0
127.90	632.0
128.90	295.0
129.90	776.0
130.90	316.0
134.90	288.0
136.80	297.0
138.90	105.0
139.90	159.0
140.90	2038.0
142.00	235.0
143.00	2742.0
143.90	177.0
144.90	962.0
145.90	270.0
147.00	143.0
147.90	539.0
149.10	138.0
149.90	183.0
152.00	104.0
152.80	140.0
154.80	589.0
156.80	296.0
158.80	296.0

Instrument :
MSVOA_V
ClientSampleId :
BFB42

160.80	259.0
170.80	308.0
171.90	2768.0
173.00	2162.0
173.90	174272.0
174.90	13075.0
175.90	169792.0
176.90	10236.0
177.90	293.0

Instrument :
MSVOA_V
ClientSampleId :
BFB42

m/z	Abundance
35.10	150.0
36.00	1447.0
37.00	7960.0
38.00	7296.0
39.00	3368.0
39.90	1159.0
43.00	178.0
44.00	1880.0
45.00	1395.0
45.90	351.0
46.90	2566.0
48.00	976.0
49.00	7204.0
50.00	33560.0
51.00	10775.0
51.90	473.0
52.90	370.0
55.00	481.0
56.00	2701.0
57.00	4588.0
58.10	230.0
60.00	1703.0
61.00	8523.0
62.00	8613.0
63.00	7617.0
64.00	1069.0
65.10	1800.0
66.10	144.0
67.00	431.0
68.00	17424.0
69.00	17576.0
70.10	1467.0
71.00	122.0
72.10	1133.0
73.00	7749.0
74.00	30352.0
75.00	88336.0
76.00	7655.0
77.00	1094.0
78.00	837.0
78.90	5751.0
79.90	1633.0
80.90	5938.0
81.90	1407.0
83.10	173.0
85.90	363.0
87.00	7888.0
88.00	7584.0
91.00	611.0
92.00	5489.0
93.00	7820.0
94.00	21432.0
95.00	180352.0
96.00	11605.0
97.00	388.0
104.00	827.0
105.00	299.0
105.90	785.0
106.90	214.0
109.90	150.0
111.10	219.0
111.80	139.0
112.70	131.0
114.90	187.0
115.90	676.0
116.90	1484.0
117.90	687.0
118.80	979.0
124.90	109.0
127.80	616.0
128.90	271.0
130.00	667.0
130.90	268.0
134.80	281.0
136.80	284.0
138.90	106.0
139.90	195.0
140.90	1865.0
142.00	226.0
143.00	2424.0
143.80	190.0
144.90	773.0
145.90	267.0
146.80	116.0
147.80	488.0
149.10	116.0
149.90	206.0
151.90	103.0
152.80	129.0
154.90	562.0
156.80	274.0
158.90	223.0

Instrument :
MSVOA_V
ClientSampleId :
BFB42

160.80	253.0
170.70	283.0
171.90	2688.0
173.00	1970.0
173.90	164288.0
174.90	11952.0
175.90	158272.0
176.90	9802.0
177.90	294.0

Instrument :
MSVOA_V
ClientSampleId :
BFB42

Scan 2793 (10.071 min): VV012922.D
BFB42

m/z	Abundance
39.90	1016.0
43.00	113.0
43.90	1018.0
44.90	139.0

Instrument :
MSVOA_V
ClientSampleId :
BFB42