
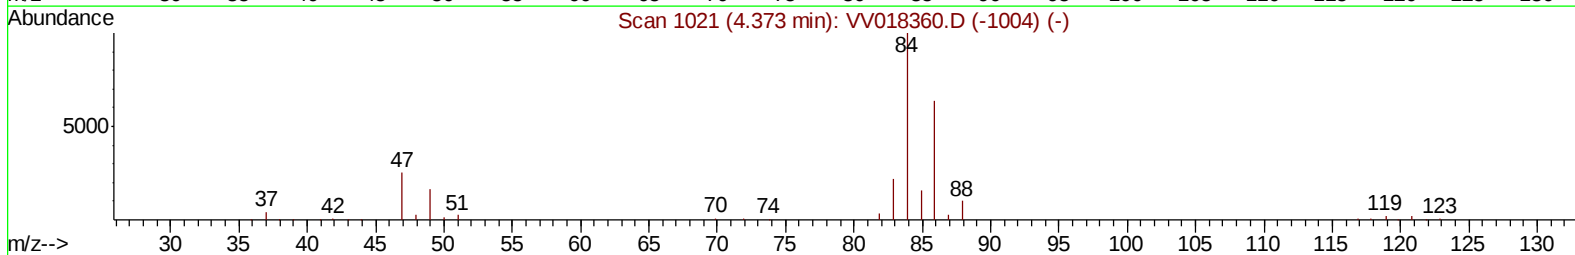
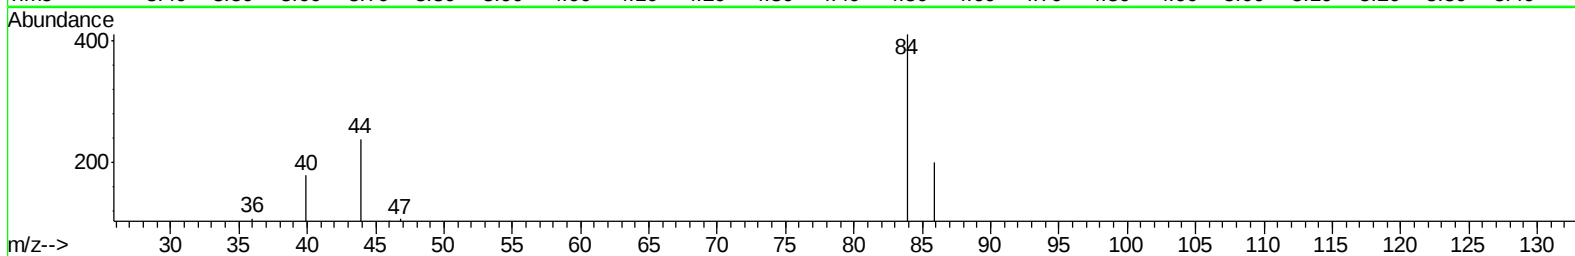


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV092120\
Data File : VV018380.D
Acq On : 21 Sep 2020 19:00
Operator : SY/MD
Sample : L4090-14
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 24 Sample Multiplier: 1

Quant Time: Sep 22 04:38:18 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Sep 22 04:28:24 2020
Response via : Initial Calibration

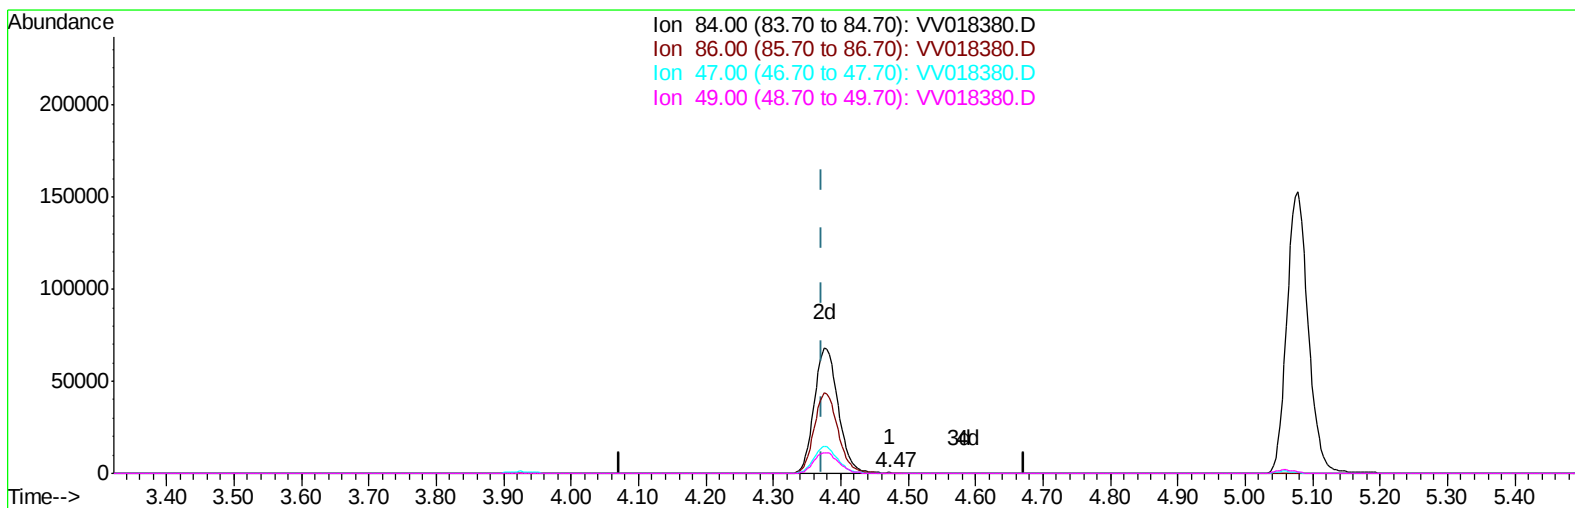

TIC: VV018380.D

(24) Chloroform-d (S)

4.473min (+0.100) 0.05ug/L

response 207

Ion	Exp%	Act%
84.00	100	100
86.00	62.40	51.21
47.00	41.10	29.95
49.00	24.20	21.26