
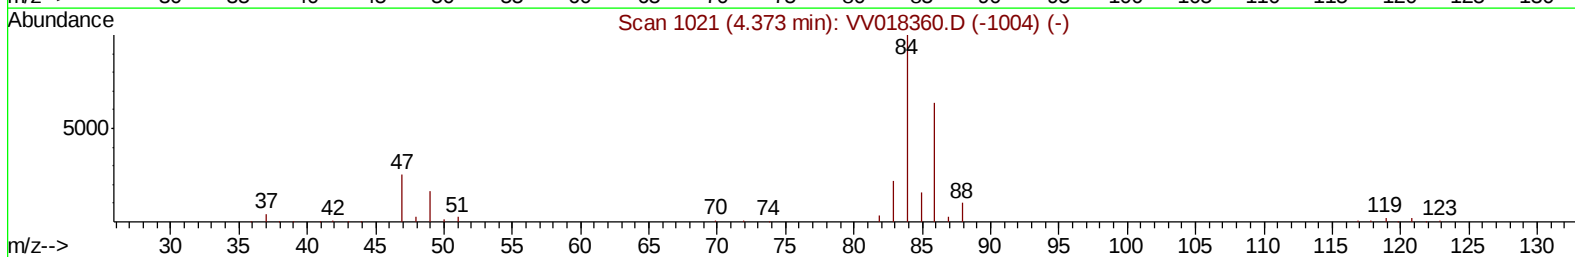
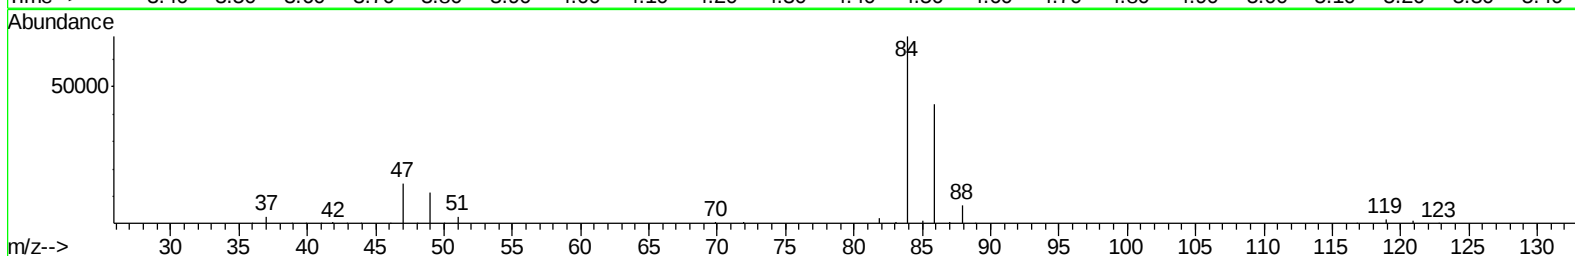


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV092120\
Data File : VV018380.D
Acq On : 21 Sep 2020 19:00
Operator : SY/MD
Sample : L4090-14
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 24 Sample Multiplier: 1

Quant Time: Sep 22 04:38:18 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Sep 22 04:28:24 2020
Response via : Initial Calibration

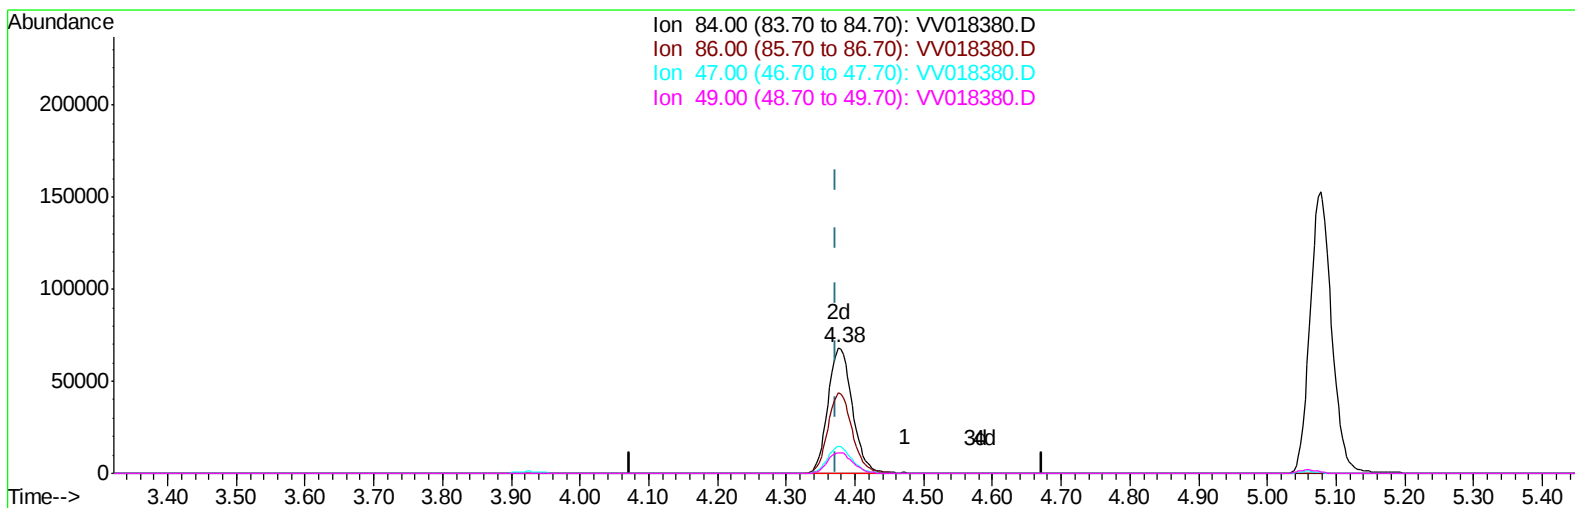

TIC: VV018380.D

(24) Chloroform-d (S)

4.376min (+0.003) 41.13ug/L m

response 167853

Ion	Exp%	Act%
84.00	100	100
86.00	62.40	0.06#
47.00	41.10	0.04#
49.00	24.20	0.03#