

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092120\
 Data File : VV018362.D
 Acq On : 21 Sep 2020 11:50
 Operator : SY/MD
 Sample : L4065-09
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AH5

Quant Time: Sep 22 04:48:04 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Sep 22 04:28:24 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	266758	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	266109	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	128069	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	98424	45.27	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	90.54%
7) Chloroethane-d5	1.58	69	82691	46.48	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	92.96%
11) 1,1-Dichloroethene-d2	2.12	63	144900	36.34	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	72.68%
21) 2-Butanone-d5	3.91	46	119271	89.63	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	89.63%
24) Chloroform-d	4.37	84	178002	47.19	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.38%
26) 1,2-Dichloroethane-d4	5.05	65	119563	49.45	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.90%
32) Benzene-d6	5.07	84	358708	47.09	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.18%
36) 1,2-Dichloropropane-d6	6.09	67	116112	47.97	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	95.94%
41) Toluene-d8	7.34	98	320342	46.14	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.28%
43) trans-1,3-Dichloropropene-	7.64	79	55954	45.49	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	90.98%
47) 2-Hexanone-d5	8.11	63	74463	81.21	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	81.21%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	129943	42.77	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	85.54%
64) 1,2-Dichlorobenzene-d4	11.65	152	132694	50.45	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	100.90%


Target Compounds					Ovalue
13) Acetone	2.19	43	7171	6.730	ug/L 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV092120\
Data File : VV018362.D
Acq On : 21 Sep 2020 11:50
Operator : SY/MD
Sample : L4065-09
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AH5

Quant Time: Sep 22 04:48:04 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Sep 22 04:28:24 2020
Response via : Initial Calibration

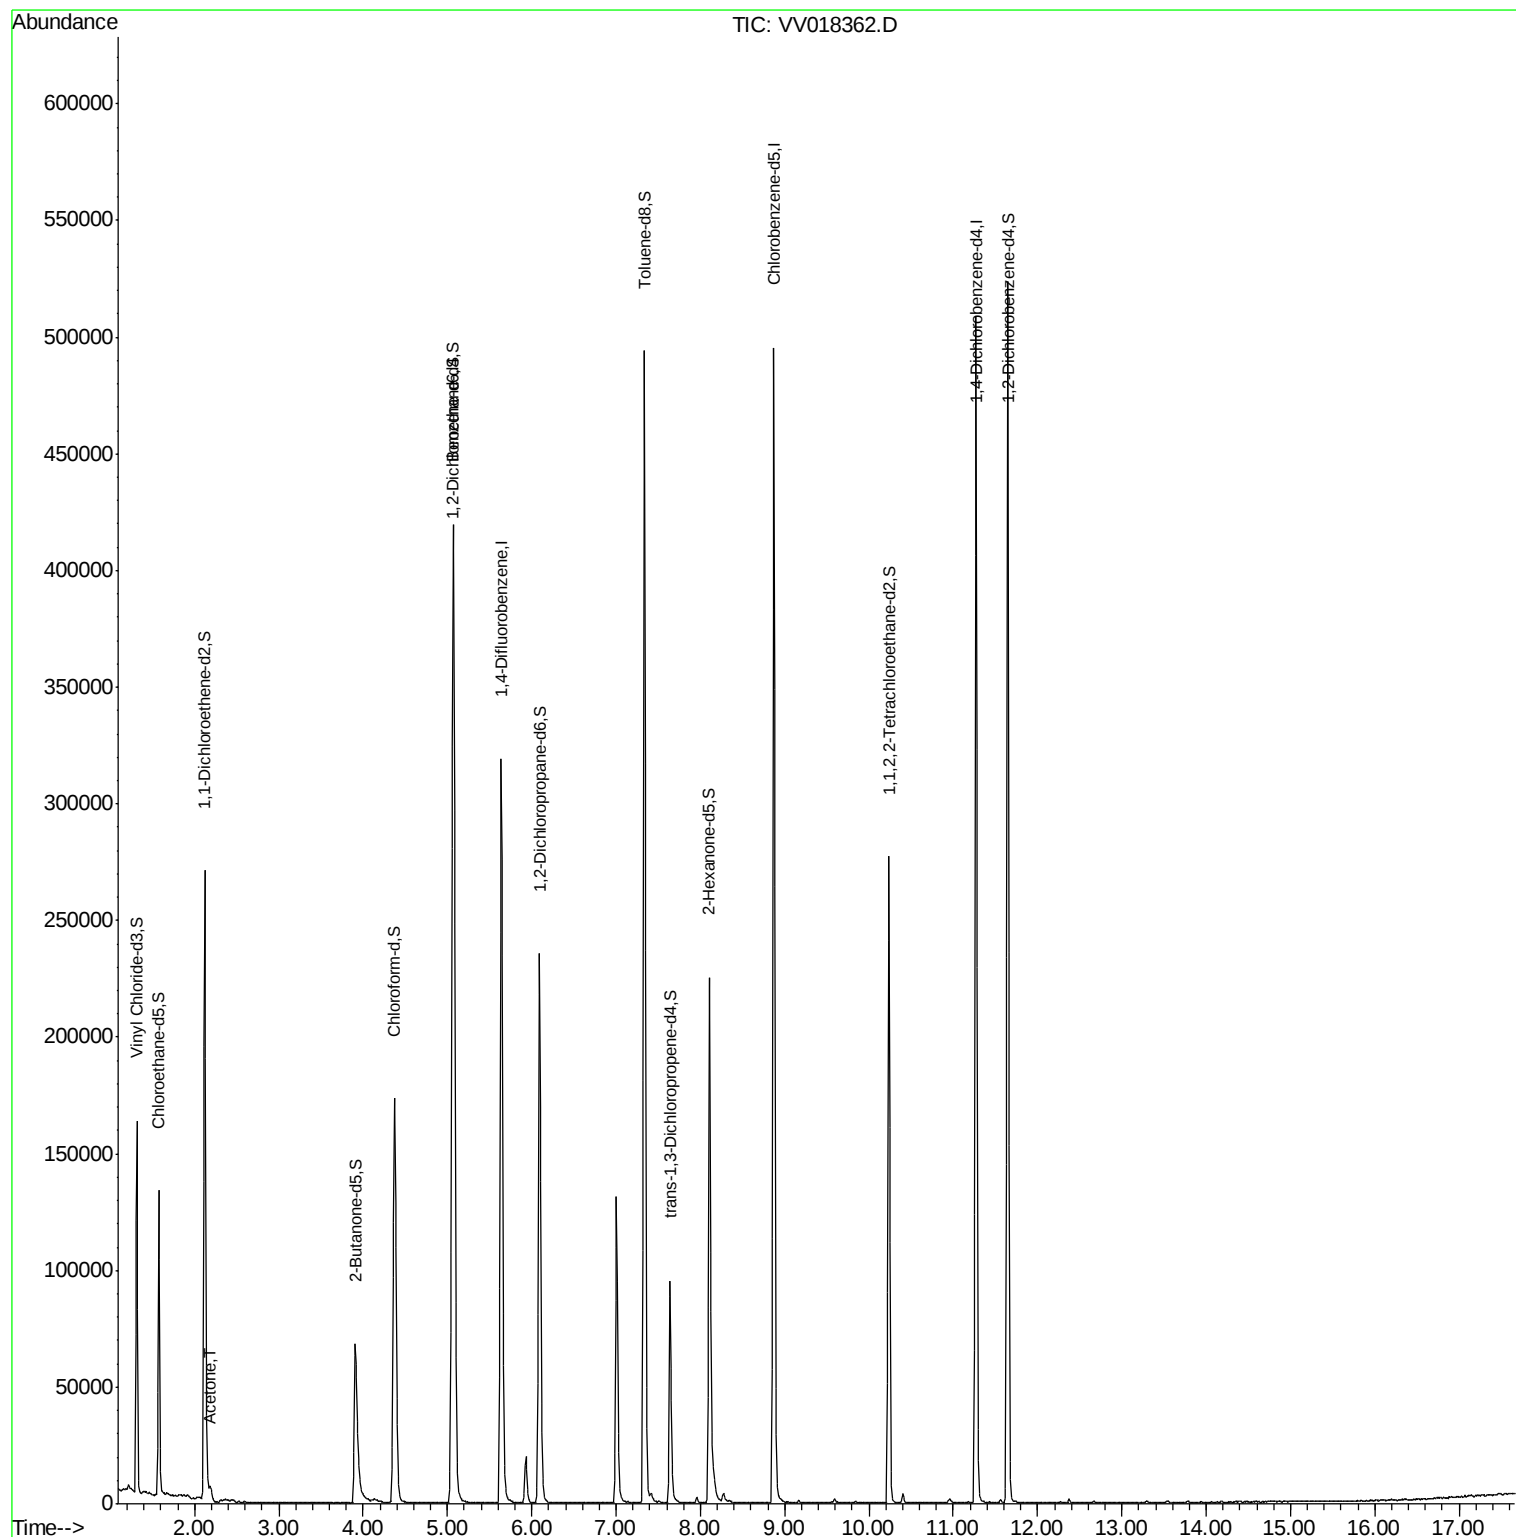

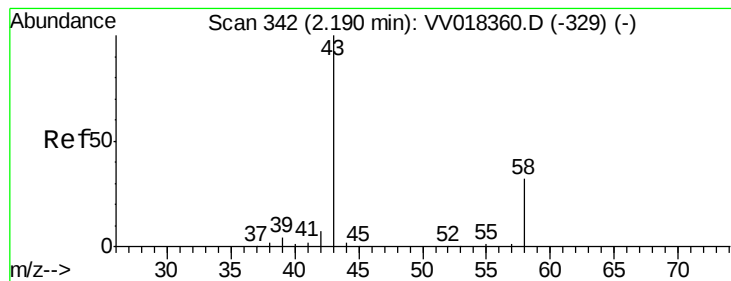

#13
 Acetone
 Concen: 6.730 ug/L
 RT: 2.19 min Scan# 341
 Delta R.T. -0.00 min
 Lab File: VV018362.D
 Acq: 21 Sep 2020 11:50

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AH5

Tot Ion: 43 Resp: 7171
 Ion Ratio Lower Upper
 43 100
 58 33.6 0.0 67.4

