

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092120\
 Data File : VV018374.D
 Acq On : 21 Sep 2020 16:45
 Operator : SY/MD
 Sample : L4090-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFWY0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.116	3	8	12	rBV	152208	134555	2.19%	0.934%
2	1.225	37	42	47	rBV	11660	11023	0.18%	0.076%
3	1.315	61	70	81	rVB2	192349	227609	3.71%	1.579%
4	1.425	100	104	111	rVB	9658	9967	0.16%	0.069%
5	1.579	144	152	165	rVB	128350	144091	2.35%	1.000%
6	1.647	167	173	183	rVB	9255	11562	0.19%	0.080%
7	1.778	207	214	221	rBV	15712	19658	0.32%	0.136%
8	1.820	222	227	241	rVB2	12826	19027	0.31%	0.132%
9	1.997	275	282	287	rBV2	5487	6951	0.11%	0.048%
10	2.032	289	293	302	rVB5	3995	5452	0.09%	0.038%
11	2.122	310	321	358	rVB	252579	394659	6.43%	2.739%
12	2.312	372	380	387	rBV2	2424	3676	0.06%	0.026%
13	2.640	479	482	489	rVB3	242	204	0.00%	0.001%
14	2.685	492	496	498	rBV3	217	200	0.00%	0.001%
15	2.737	510	512	516	rVB	307	147	0.00%	0.001%
16	2.785	516	527	536	rVB4	3277	5745	0.09%	0.040%
17	2.888	553	559	562	rBV2	244	231	0.00%	0.002%
18	2.978	577	587	599	rVV3	3732	6896	0.11%	0.048%
19	3.068	606	615	625	rVB5	2201	4544	0.07%	0.032%
20	3.222	656	663	664	rBV2	344	309	0.01%	0.002%
21	3.245	667	670	674	rVB2	222	156	0.00%	0.001%
22	3.383	708	713	715	rBV2	200	134	0.00%	0.001%
23	3.486	738	745	753	rBV4	804	1316	0.02%	0.009%
24	3.923	868	881	919	rBV4	69142	245938	4.01%	1.707%
25	4.376	1004	1022	1051	rBV	164193	401451	6.54%	2.786%
26	4.508	1062	1063	1067	rVB	290	141	0.00%	0.001%
27	4.550	1074	1076	1082	rVB2	336	273	0.00%	0.002%
28	4.698	1116	1122	1125	rBV4	684	851	0.01%	0.006%
29	4.733	1131	1133	1138	rVB2	285	212	0.00%	0.001%
30	4.785	1144	1149	1152	rBV3	543	665	0.01%	0.005%
31	4.942	1189	1198	1203	rBV4	646	927	0.02%	0.006%
32	5.074	1221	1239	1275	rBV2	398483	1026287	16.72%	7.121%
33	5.367	1327	1330	1332	rBV2	202	152	0.00%	0.001%
34	5.415	1335	1345	1349	rVV6	916	1173	0.02%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092120\
 Data File : VV018374.D
 Acq On : 21 Sep 2020 16:45
 Operator : SY/MD
 Sample : L4090-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFWY0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Title : VOC Analysis

35	5.518	1374	1377	1383	rBV3	526	601	0.01%	0.004%
36	5.569	1390	1393	1395	rBV	203	154	0.00%	0.001%
37	5.643	1403	1416	1443	rBV	321283	637527	10.39%	4.424%
38	5.936	1492	1507	1540	rVV	3204566	6136413	100.00%	42.581%
39	6.093	1544	1556	1586	rVB	231213	470396	7.67%	3.264%
40	6.286	1614	1616	1619	rBV3	356	234	0.00%	0.002%
41	6.511	1683	1686	1691	rVB2	289	264	0.00%	0.002%
42	6.601	1708	1714	1715	rBV2	607	510	0.01%	0.004%
43	6.653	1726	1730	1733	rBV2	172	148	0.00%	0.001%
44	6.669	1733	1735	1740	rVB2	171	132	0.00%	0.001%
45	6.804	1774	1777	1780	rVB2	259	158	0.00%	0.001%
46	7.007	1829	1840	1867	rBV	129985	233725	3.81%	1.622%
47	7.158	1885	1887	1892	rBV3	286	186	0.00%	0.001%
48	7.254	1914	1917	1919	rBV	398	260	0.00%	0.002%
49	7.338	1930	1943	1966	rBV	474275	815718	13.29%	5.660%
50	7.550	2006	2009	2012	rVB2	220	138	0.00%	0.001%
51	7.585	2018	2020	2023	rVB	350	167	0.00%	0.001%
52	7.643	2028	2038	2058	rBV	94211	161800	2.64%	1.123%
53	7.878	2107	2111	2115	rVB3	248	186	0.00%	0.001%
54	7.961	2129	2137	2143	rBV2	693	1130	0.02%	0.008%
55	8.000	2143	2149	2161	rVB4	1929	2902	0.05%	0.020%
56	8.109	2172	2183	2214	rBV	226267	416760	6.79%	2.892%
57	8.402	2270	2274	2276	rBV	170	132	0.00%	0.001%
58	8.453	2287	2290	2292	rVV	183	157	0.00%	0.001%
59	8.592	2330	2333	2335	rBV	180	150	0.00%	0.001%
60	8.817	2400	2403	2409	rVB2	310	276	0.00%	0.002%
61	8.871	2409	2420	2442	rBV	493397	796313	12.98%	5.526%
62	9.035	2468	2471	2473	rBV3	588	442	0.01%	0.003%
63	9.576	2631	2639	2644	rBV3	988	1511	0.02%	0.010%
64	9.955	2751	2757	2765	rVB3	862	1052	0.02%	0.007%
65	10.238	2832	2845	2866	rBV	282094	443555	7.23%	3.078%
66	10.405	2888	2897	2905	rVB2	1584	2196	0.04%	0.015%
67	10.563	2940	2946	2953	rBV2	724	1043	0.02%	0.007%
68	10.617	2959	2963	2966	rBV	172	134	0.00%	0.001%
69	10.749	3001	3004	3012	rVB	183	162	0.00%	0.001%
70	10.942	3057	3064	3071	rVB	757	1089	0.02%	0.008%
71	11.119	3114	3119	3128	rVB2	503	651	0.01%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092120\
 Data File : VV018374.D
 Acq On : 21 Sep 2020 16:45
 Operator : SY/MD
 Sample : L4090-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFWY0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Title : VOC Analysis

72	11.161	3128	3132	3134	rBV	166	134	0.00%	0.001%
73	11.177	3134	3137	3141	rVB3	578	433	0.01%	0.003%
74	11.209	3141	3147	3154	rBV3	1498	2058	0.03%	0.014%
75	11.270	3154	3166	3190	rBV	511090	781078	12.73%	5.420%
76	11.463	3223	3226	3228	rVB	232	152	0.00%	0.001%
77	11.563	3250	3257	3260	rBV4	1626	1795	0.03%	0.012%
78	11.646	3271	3283	3301	rBV	502235	783663	12.77%	5.438%
79	11.826	3336	3339	3344	rVB3	386	312	0.01%	0.002%
80	11.855	3344	3348	3351	rBV3	172	155	0.00%	0.001%
81	11.894	3356	3360	3362	rBV3	236	179	0.00%	0.001%
82	12.270	3473	3477	3483	rBV3	346	392	0.01%	0.003%
83	12.325	3491	3494	3499	rVB	327	273	0.00%	0.002%
84	12.373	3499	3509	3517	rBV5	1687	2166	0.04%	0.015%
85	12.456	3531	3535	3539	rVB2	419	295	0.00%	0.002%
86	12.482	3539	3543	3549	rBV2	224	290	0.00%	0.002%
87	12.608	3578	3582	3586	rBV3	234	190	0.00%	0.001%
88	12.672	3594	3602	3610	rBV3	2277	3564	0.06%	0.025%
89	13.289	3786	3794	3803	rBV4	3502	4974	0.08%	0.035%
90	13.530	3861	3869	3885	rBV	4061	6336	0.10%	0.044%
91	13.688	3915	3918	3921	rBV2	176	143	0.00%	0.001%
92	13.768	3936	3943	3953	rVB3	3883	5934	0.10%	0.041%
93	13.823	3958	3960	3966	rVB2	306	306	0.00%	0.002%
94	13.852	3966	3969	3973	rBV	215	179	0.00%	0.001%
95	13.952	3997	4000	4003	rBV	285	209	0.00%	0.001%
96	14.103	4043	4047	4049	rBV3	228	169	0.00%	0.001%
97	14.164	4060	4066	4067	rBV2	272	249	0.00%	0.002%
98	14.273	4095	4100	4104	rBV3	263	323	0.01%	0.002%
99	14.656	4215	4219	4227	rBV3	229	435	0.01%	0.003%
100	14.730	4238	4242	4247	rBV2	390	357	0.01%	0.002%


Sum of corrected areas: 14411297

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV092120\
Data File : VV018374.D
Acq On : 21 Sep 2020 16:45
Operator : SY/MD
Sample : L4090-08
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFWY0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

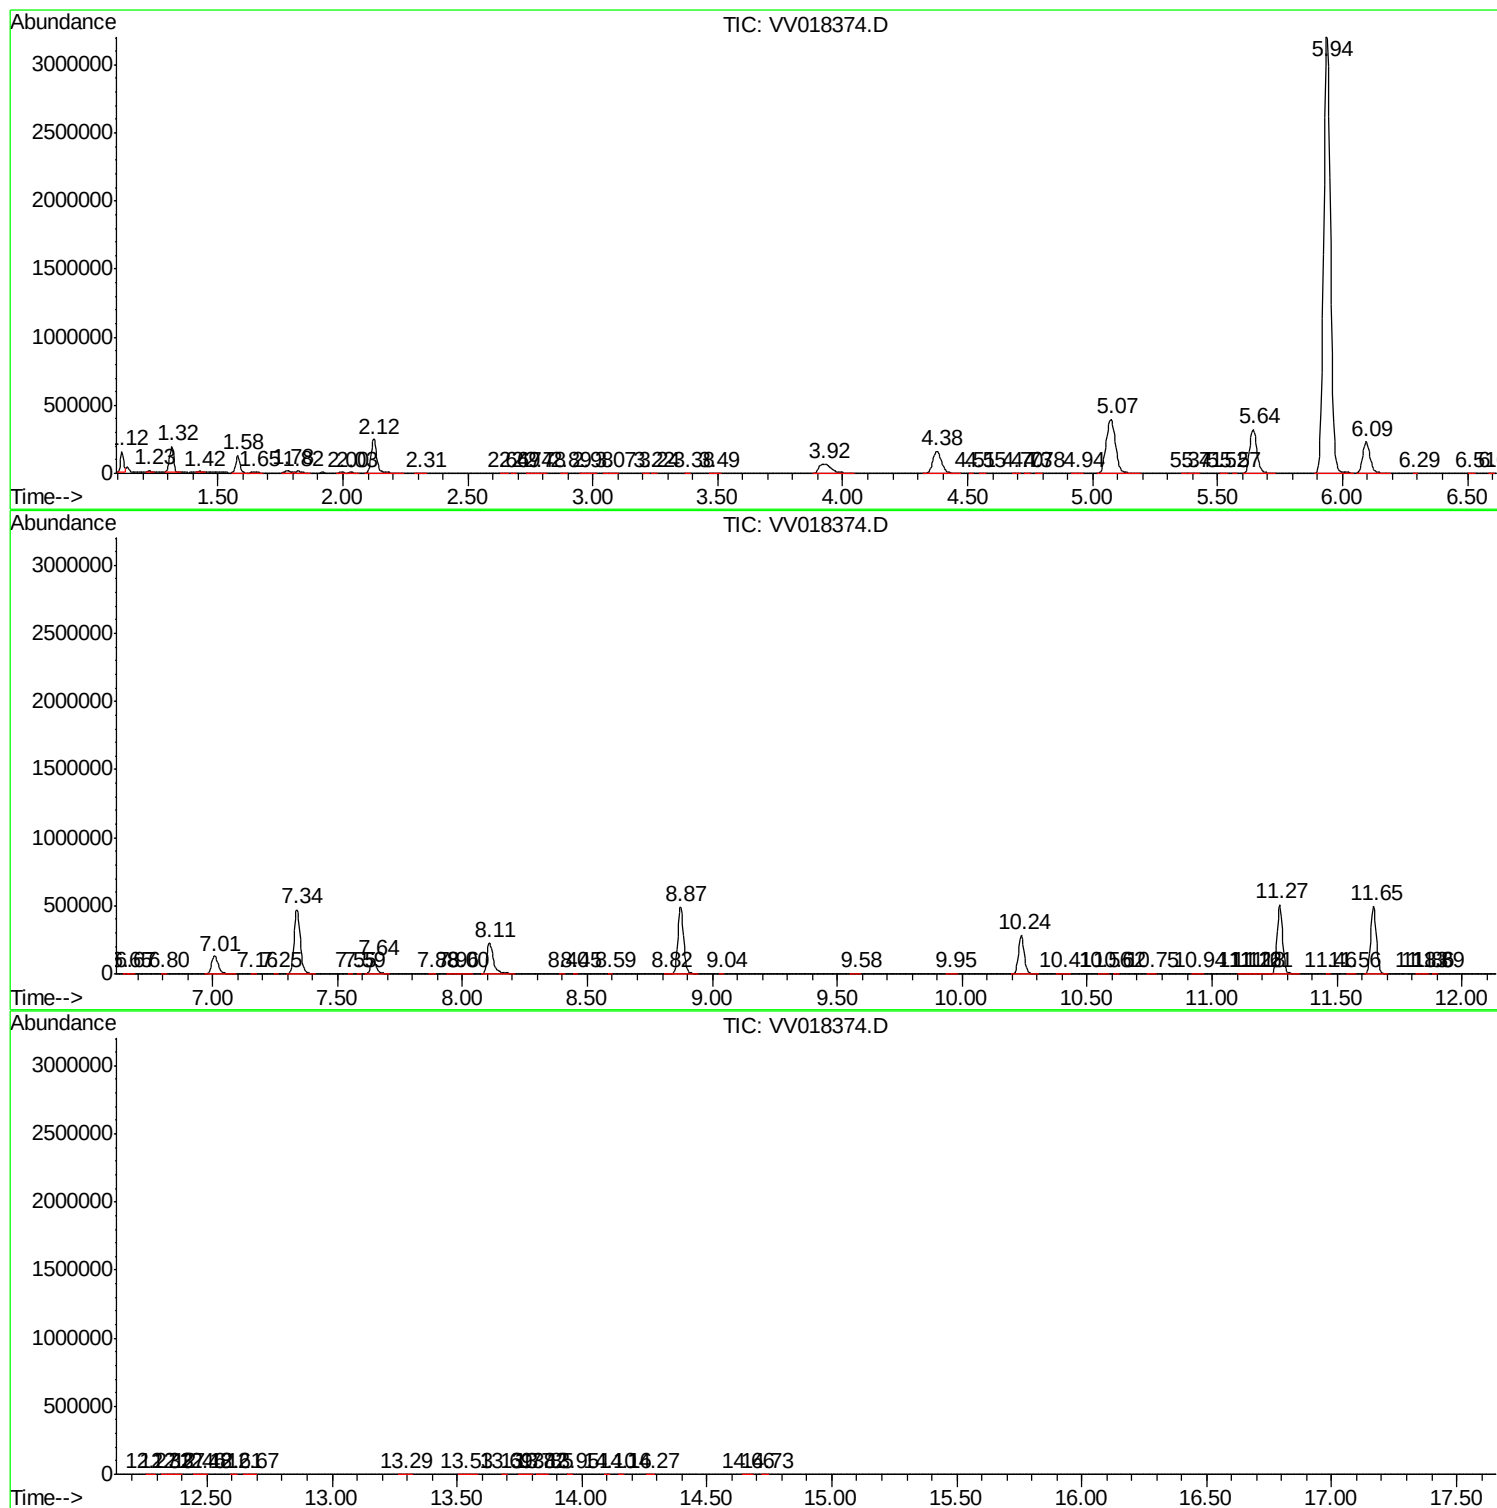

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV092120\
Data File : VV018374.D
Acq On : 21 Sep 2020 16:45
Operator : SY/MD
Sample : L4090-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFWY0

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV092120\
Data File : VV018374.D
Acq On : 21 Sep 2020 16:45
Operator : SY/MD
Sample : L4090-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFWY0

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc