

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092120\
 Data File : VV018381.D
 Acq On : 21 Sep 2020 19:23
 Operator : SY/MD
 Sample : L4092-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFX02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	84	rVB	136152	135961	13.59%	1.796%
2	1.579	145	152	162	rBV	117560	130940	13.09%	1.730%
3	2.123	311	321	354	rVB	238210	366749	36.66%	4.845%
4	2.602	468	470	472	rBV	264	151	0.02%	0.002%
5	2.688	495	497	499	rBV	170	120	0.01%	0.002%
6	2.872	549	554	561	rBV2	129	195	0.02%	0.003%
7	2.913	566	567	571	rVB	145	41	0.00%	0.001%
8	2.955	575	580	583	rBV2	129	141	0.01%	0.002%
9	3.167	642	646	647	rBV	82	68	0.01%	0.001%
10	3.190	651	653	658	rVB	159	130	0.01%	0.002%
11	3.219	658	662	665	rBV2	66	55	0.01%	0.001%
12	3.293	679	685	687	rBV2	74	75	0.01%	0.001%
13	3.376	709	711	713	rVV2	101	50	0.00%	0.001%
14	3.412	719	722	724	rBV2	103	69	0.01%	0.001%
15	3.470	737	740	742	rBV	89	53	0.01%	0.001%
16	3.512	750	753	755	rBV2	82	59	0.01%	0.001%
17	3.563	764	769	771	rBV2	121	101	0.01%	0.001%
18	3.595	776	779	782	rBV	101	63	0.01%	0.001%
19	3.647	792	795	801	rVB2	154	162	0.02%	0.002%
20	3.676	801	804	806	rBV	130	86	0.01%	0.001%
21	3.704	810	813	816	rVV	83	56	0.01%	0.001%
22	3.724	816	819	822	rVB2	101	65	0.01%	0.001%
23	3.749	822	827	832	rBV2	94	110	0.01%	0.001%
24	3.788	835	839	848	rVB2	325	425	0.04%	0.006%
25	3.913	862	878	909	rBV	62305	185942	18.59%	2.456%
26	4.376	1006	1022	1055	rBV	161174	393271	39.31%	5.195%
27	4.592	1086	1089	1090	rBV	153	73	0.01%	0.001%
28	4.598	1090	1091	1094	rVV2	217	80	0.01%	0.001%
29	4.640	1101	1104	1107	rVB2	194	80	0.01%	0.001%
30	4.659	1107	1110	1115	rVB2	74	65	0.01%	0.001%
31	4.685	1115	1118	1121	rBV2	123	91	0.01%	0.001%
32	4.711	1124	1126	1131	rBV2	145	80	0.01%	0.001%
33	4.804	1152	1155	1157	rBV2	95	63	0.01%	0.001%
34	4.881	1176	1179	1182	rVB2	65	41	0.00%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092120\
 Data File : VV018381.D
 Acq On : 21 Sep 2020 19:23
 Operator : SY/MD
 Sample : L4092-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFX02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Title : VOC Analysis

35	5.074	1222	1239	1281	rBV2	390979	1000478	100.00%	13.217%
36	5.396	1337	1339	1342	rBV2	161	117	0.01%	0.002%
37	5.482	1363	1366	1372	rVB	101	84	0.01%	0.001%
38	5.511	1372	1375	1380	rBV2	131	136	0.01%	0.002%
39	5.550	1385	1387	1389	rBV2	95	52	0.01%	0.001%
40	5.643	1403	1416	1439	rBV	303131	600349	60.01%	7.931%
41	5.933	1493	1506	1528	rVB4	29606	66723	6.67%	0.881%
42	6.093	1543	1556	1586	rBV	223761	453144	45.29%	5.986%
43	6.238	1598	1601	1607	rBV3	608	631	0.06%	0.008%
44	6.306	1617	1622	1624	rBV2	65	65	0.01%	0.001%
45	6.364	1637	1640	1642	rBV	66	47	0.00%	0.001%
46	6.380	1642	1645	1649	rVB	159	103	0.01%	0.001%
47	6.405	1649	1653	1656	rBV	111	82	0.01%	0.001%
48	6.473	1671	1674	1675	rBV	90	53	0.01%	0.001%
49	6.537	1691	1694	1698	rBV2	84	63	0.01%	0.001%
50	6.601	1708	1714	1718	rBV4	659	852	0.09%	0.011%
51	6.701	1742	1745	1751	rVB2	69	60	0.01%	0.001%
52	6.785	1768	1771	1774	rVB	214	130	0.01%	0.002%
53	6.807	1774	1778	1780	rBV	85	66	0.01%	0.001%
54	6.894	1802	1805	1807	rBV	87	48	0.00%	0.001%
55	7.007	1829	1840	1866	rBV	123022	220416	22.03%	2.912%
56	7.164	1881	1889	1897	rVB8	1357	2423	0.24%	0.032%
57	7.199	1898	1900	1904	rVB	231	154	0.02%	0.002%
58	7.222	1904	1907	1910	rBV	98	58	0.01%	0.001%
59	7.338	1931	1943	1971	rBV	461084	785461	78.51%	10.377%
60	7.643	2027	2038	2062	rBV	89143	153413	15.33%	2.027%
61	7.791	2081	2084	2086	rBV	278	123	0.01%	0.002%
62	7.820	2091	2093	2095	rVB2	262	99	0.01%	0.001%
63	7.916	2117	2123	2127	rBV2	126	130	0.01%	0.002%
64	7.958	2127	2136	2144	rVV2	713	1205	0.12%	0.016%
65	8.007	2149	2151	2152	rBV2	111	47	0.00%	0.001%
66	8.071	2166	2171	2173	rBV2	73	75	0.01%	0.001%
67	8.109	2173	2183	2226	rBV2	210997	409187	40.90%	5.406%
68	8.351	2256	2258	2262	rVB2	324	129	0.01%	0.002%
69	8.470	2290	2295	2297	rBV2	104	104	0.01%	0.001%
70	8.511	2305	2308	2312	rBV2	222	150	0.01%	0.002%
71	8.875	2408	2421	2457	rBV	477852	763011	76.26%	10.080%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092120\
 Data File : VV018381.D
 Acq On : 21 Sep 2020 19:23
 Operator : SY/MD
 Sample : L4092-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFX02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Title : VOC Analysis

72	9.077	2483	2484	2487	rVB	140	68	0.01%	0.001%
73	9.119	2495	2497	2503	rVB	189	114	0.01%	0.002%
74	9.148	2503	2506	2508	rBV	213	145	0.01%	0.002%
75	9.212	2523	2526	2528	rBV	116	71	0.01%	0.001%
76	9.283	2546	2548	2551	rBV	76	42	0.00%	0.001%
77	9.299	2551	2553	2556	rBV	117	81	0.01%	0.001%
78	9.383	2576	2579	2582	rBV	170	115	0.01%	0.002%
79	9.473	2604	2607	2609	rBV2	91	48	0.00%	0.001%
80	9.572	2636	2638	2641	rBV	192	81	0.01%	0.001%
81	9.736	2685	2689	2691	rBV2	130	103	0.01%	0.001%
82	9.974	2760	2763	2767	rBV2	76	59	0.01%	0.001%
83	10.238	2832	2845	2861	rBV	254197	400277	40.01%	5.288%
84	10.341	2875	2877	2878	rBV	145	69	0.01%	0.001%
85	10.402	2889	2896	2904	rVB2	1061	1657	0.17%	0.022%
86	10.466	2913	2916	2923	rBV2	141	135	0.01%	0.002%
87	10.540	2935	2939	2942	rBV	127	95	0.01%	0.001%
88	10.746	3000	3003	3004	rBV	138	73	0.01%	0.001%
89	10.858	3035	3038	3042	rBV2	120	114	0.01%	0.002%
90	10.939	3061	3063	3065	rBV	101	56	0.01%	0.001%
91	11.206	3144	3146	3150	rBV2	233	200	0.02%	0.003%
92	11.270	3154	3166	3192	rVV	475391	720454	72.01%	9.518%
93	11.563	3250	3257	3260	rBV3	1053	1225	0.12%	0.016%
94	11.646	3270	3283	3304	rBV	496909	766140	76.58%	10.121%
95	11.826	3336	3339	3343	rVB2	343	242	0.02%	0.003%
96	11.887	3356	3358	3361	rBV	182	79	0.01%	0.001%
97	12.373	3503	3509	3516	rVB2	1957	2258	0.23%	0.030%
98	12.672	3600	3602	3604	rBV	247	125	0.01%	0.002%
99	13.196	3763	3765	3766	rBV	180	65	0.01%	0.001%
100	13.546	3873	3874	3877	rBV2	236	121	0.01%	0.002%


Sum of corrected areas: 7569491

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV092120\
Data File : VV018381.D
Acq On : 21 Sep 2020 19:23
Operator : SY/MD
Sample : L4092-03
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFX02

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

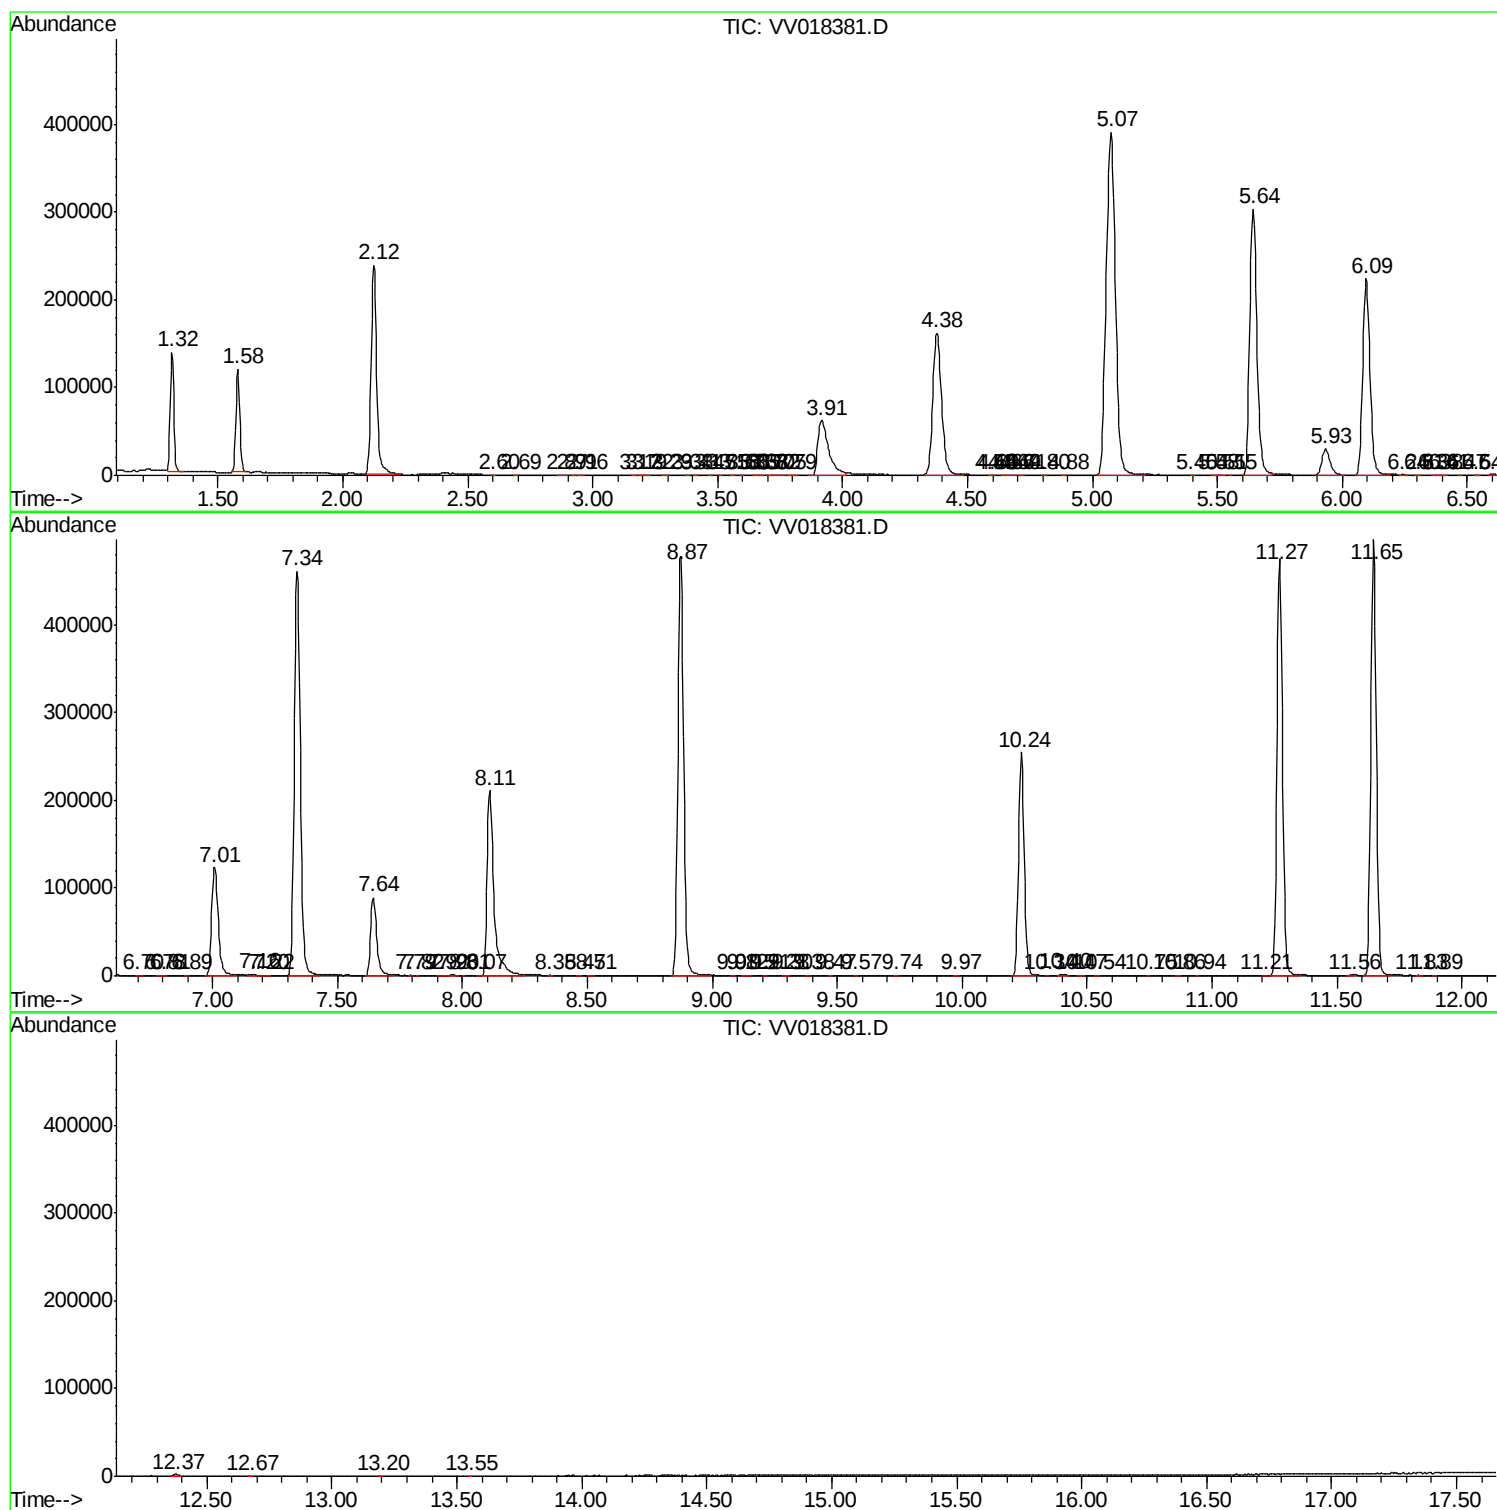

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV092120\
Data File : VV018381.D
Acq On : 21 Sep 2020 19:23
Operator : SY/MD
Sample : L4092-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFX02

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV092120\
Data File : VV018381.D
Acq On : 21 Sep 2020 19:23
Operator : SY/MD
Sample : L4092-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFX02

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc