


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV092120\
 Data File : VV018359.D
 Acq On : 21 Sep 2020 09:38
 Operator : SY/MD
 Sample : BFB95
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB95

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Title : VOC Analysis
 Last Update : Tue Sep 22 04:28:24 2020

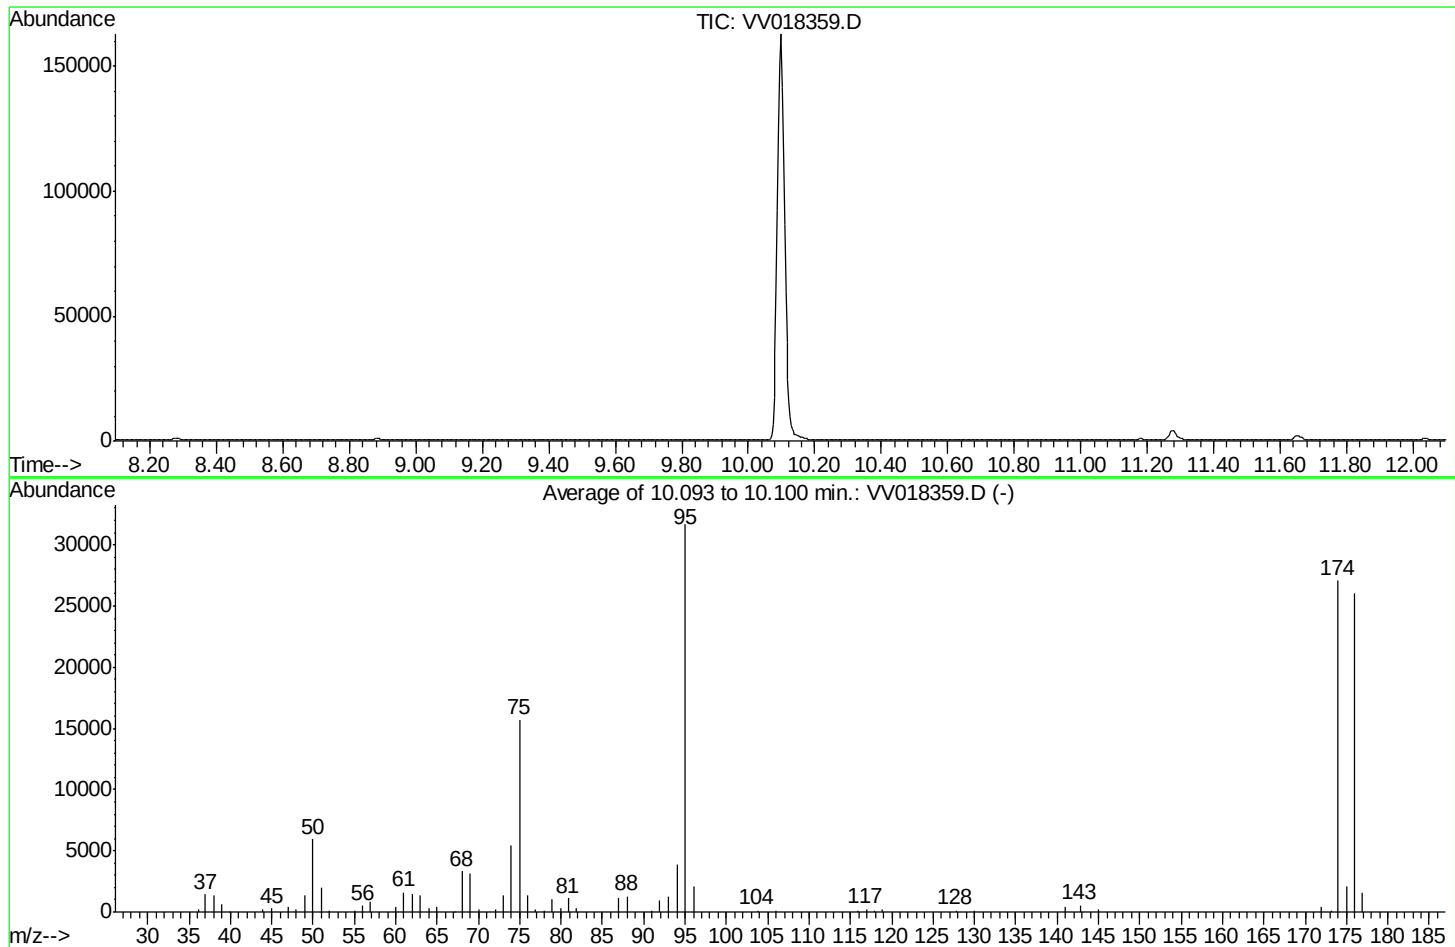

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2790

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	5948	PASS
75	95	30	80	49.6	15723	PASS
95	95	100	100	100.0	31672	PASS
96	95	5	9	6.7	2110	PASS
173	174	0.00	2	0.6	150	PASS
174	95	50	120	85.4	27053	PASS
175	174	5	9	7.8	2123	PASS
176	174	95	101	96.4	26072	PASS
177	176	5	9	6.2	1615	PASS

m/z	Abundance
36.10	237.0
37.00	1478.0
38.00	1359.0
39.00	603.0
39.90	162.0
44.00	466.0
45.00	270.0
47.00	334.0
48.00	225.0
49.00	1343.0
50.00	5826.0
51.00	1953.0
51.90	109.0
55.00	119.0
56.00	480.0
57.00	835.0
59.90	384.0
61.00	1457.0
62.00	1430.0
63.00	1366.0
64.00	272.0
65.00	328.0
67.10	116.0
68.00	3207.0
69.00	3072.0
70.00	256.0
72.00	230.0
73.00	1335.0
74.00	5263.0
75.00	15268.0
76.00	1266.0
77.00	178.0
77.90	127.0
78.90	1001.0
79.90	328.0
80.90	1059.0
81.80	295.0
87.00	1140.0
88.00	1244.0
90.90	114.0
91.90	922.0
93.00	1336.0
94.00	3706.0
95.00	29952.0
96.00	2091.0
103.70	125.0
106.00	126.0
115.90	116.0
116.90	223.0
118.00	163.0
118.80	177.0
127.80	135.0
129.90	151.0
140.90	378.0
142.80	478.0
144.90	226.0
171.90	384.0
173.90	25584.0
175.00	1961.0
175.90	24072.0
176.90	1540.0

Instrument :
MSVOA_V
ClientSampleId :
BFB95

m/z	Abundance
36.10	253.0
37.00	1489.0
38.00	1417.0
39.00	629.0
39.90	166.0
44.00	477.0
45.00	286.0
47.00	374.0
48.00	220.0
49.00	1364.0
50.00	6108.0
51.00	2049.0
51.90	110.0
55.00	139.0
56.00	516.0
56.90	885.0
60.00	412.0
61.00	1635.0
62.00	1491.0
63.00	1444.0
64.00	283.0
65.00	390.0
68.00	3414.0
69.00	3245.0
70.00	274.0
72.00	213.0
73.00	1421.0
74.00	5630.0
75.00	16233.0
76.00	1352.0
76.90	184.0
78.00	151.0
78.90	1136.0
79.90	372.0
80.90	1170.0
81.80	324.0
86.90	1237.0
88.00	1338.0
90.90	120.0
92.00	995.0
93.00	1334.0
94.00	4014.0
95.00	32728.0
96.00	2193.0
103.80	147.0
105.90	136.0
115.90	124.0
116.90	245.0
118.00	167.0
118.80	180.0
127.80	143.0
129.90	143.0
140.90	382.0
142.80	549.0
144.90	225.0
171.90	432.0
174.00	28008.0
175.00	2230.0
175.90	27072.0
177.00	1635.0

Instrument :
MSVOA_V
ClientSampleId :
BFB95

m/z	Abundance
36.10	263.0
37.00	1365.0
38.00	1369.0
39.00	594.0
39.90	179.0
44.00	476.0
45.00	265.0
47.00	403.0
48.00	185.0
49.00	1269.0
50.00	5910.0
51.00	1945.0
52.00	115.0
55.00	112.0
56.00	509.0
57.00	838.0
60.00	379.0
61.00	1630.0
62.00	1412.0
63.00	1355.0
64.00	257.0
65.00	398.0
68.00	3342.0
69.00	3125.0
70.00	265.0
72.00	174.0
73.00	1397.0
74.00	5300.0
75.00	15669.0
76.00	1357.0
76.90	190.0
78.00	165.0
78.90	1139.0
79.90	360.0
80.90	1170.0
81.80	295.0
86.90	1220.0
87.90	1320.0
90.90	127.0
92.00	957.0
93.00	1243.0
94.00	3845.0
95.00	32336.0
96.00	2048.0
103.90	163.0
105.90	117.0
115.90	121.0
116.90	234.0
117.90	144.0
118.80	175.0
127.80	140.0
130.00	122.0
140.90	364.0
142.80	548.0
145.00	218.0
171.90	478.0
173.10	452.0
174.00	27568.0
175.00	2178.0
175.90	27072.0
177.00	1671.0

Instrument :
MSVOA_V
ClientSampleId :
BFB95

Scan 2790 (10.061 min): VV018359.D
BFB95

m/z	Abundance
39.90	153.0
43.90	304.0

Instrument :
MSVOA_V
ClientSampleId :
BFB95