


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092121\
 Data File : VV022266.D
 Acq On : 21 Sep 2021 09:39
 Operator : SY/MD
 Sample : BFB234
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB234

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis
 Last Update : Wed Sep 22 01:12:58 2021

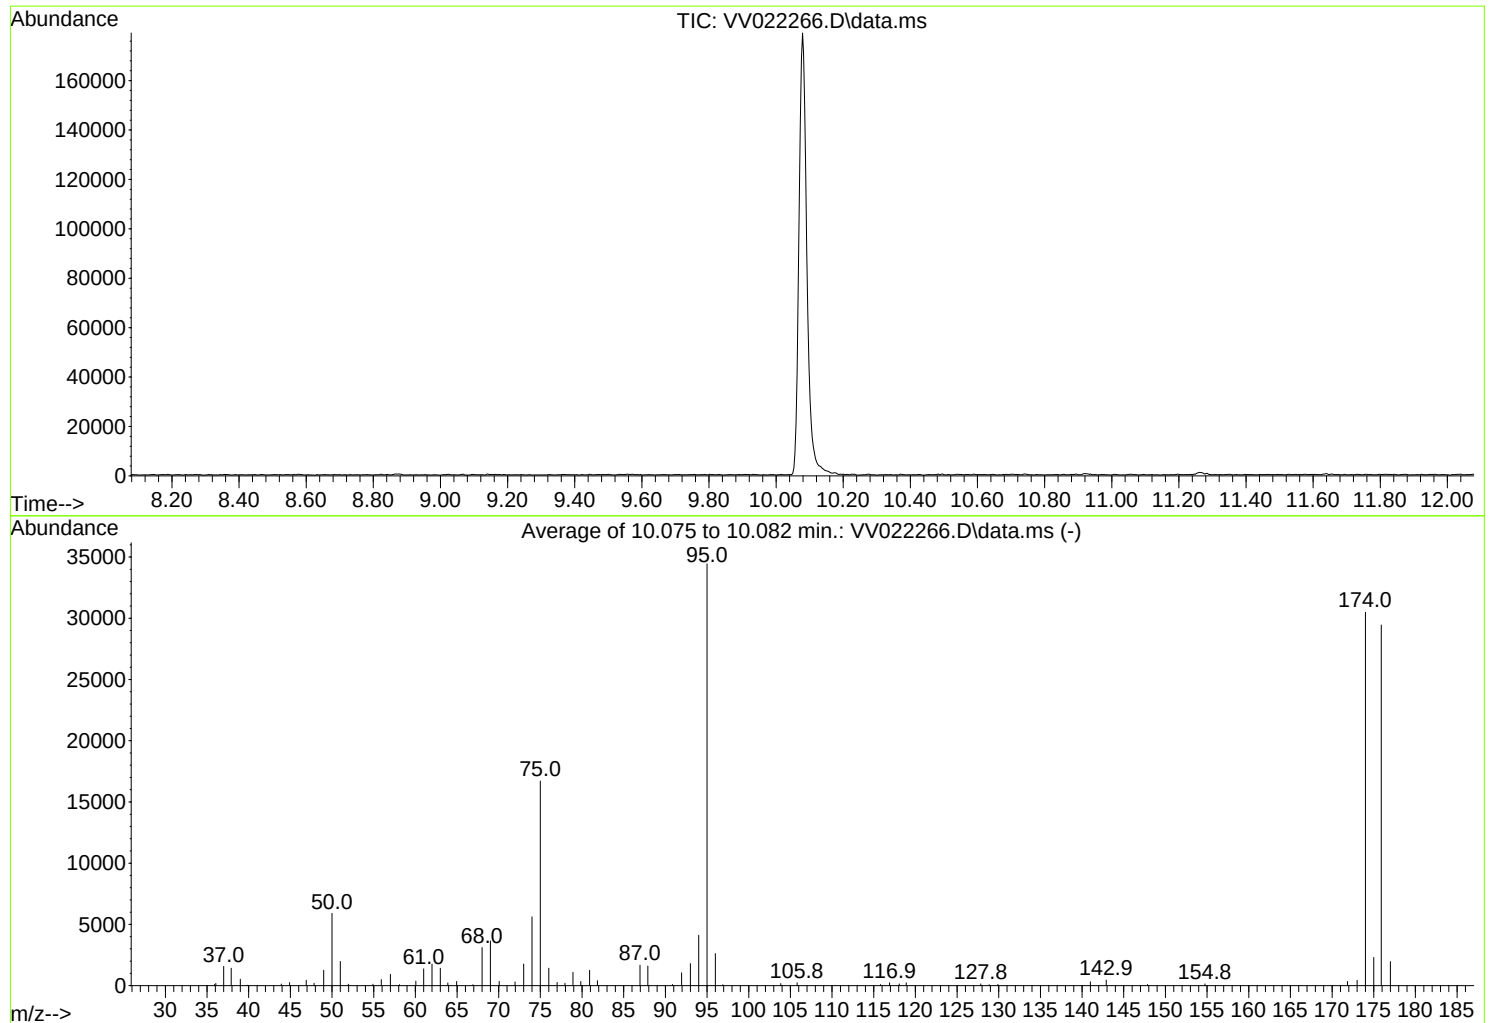

AutoFind: Scans 2810, 2811, 2812; Background Corrected with Scan 2800

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	5905	PASS
75	95	30	80	48.5	16706	PASS
95	95	100	100	100.0	34445	PASS
96	95	5	9	7.6	2608	PASS
173	174	0.00	2	1.4	429	PASS
174	95	50	120	88.5	30491	PASS
175	174	5	9	7.6	2306	PASS
176	174	95	105	96.6	29448	PASS
177	176	5	10	6.7	1959	PASS

Scan 2800 (10.043 min): VV022266.D\data.ms
BFB234

m/z	Abundance
40.00	206.0
43.90	329.0

Instrument :
MSVOA_V
ClientSampleId :
BFB234

m/z	Abundance
35.90	257.0
37.00	1588.0
37.90	1359.0
39.00	546.0
39.80	249.0
44.00	476.0
44.90	276.0
46.90	485.0
47.90	200.0
49.00	1266.0
50.00	5851.0
51.00	1956.0
52.00	106.0
54.90	131.0
55.90	496.0
57.00	924.0
60.10	384.0
61.00	1289.0
62.00	1732.0
63.00	1355.0
63.90	200.0
64.90	334.0
66.90	137.0
68.00	3066.0
69.00	3543.0
70.10	340.0
72.00	282.0
73.00	1799.0
74.00	5483.0
75.00	16382.0
76.00	1417.0
77.00	307.0
77.90	231.0
78.90	1001.0
79.90	301.0
80.90	1287.0
81.90	385.0
87.00	1672.0
87.90	1644.0
92.00	1022.0
93.00	1838.0
94.00	4134.0
95.00	33680.0
96.00	2492.0
96.90	125.0
103.90	135.0
105.80	238.0
115.80	149.0
116.90	248.0
118.10	115.0
118.80	242.0
127.80	120.0
141.00	314.0
142.90	411.0
154.80	132.0
171.90	368.0
173.00	427.0
174.00	29392.0
175.00	2156.0
175.90	28360.0
177.00	1881.0

Instrument :
MSVOA_V
ClientSampleId :
BFB234

m/z	Abundance
36.10	272.0
37.00	1629.0
37.90	1486.0
39.00	540.0
39.90	255.0
43.90	457.0
44.90	270.0
46.90	442.0
47.90	202.0
49.00	1308.0
50.00	6105.0
51.00	2036.0
52.00	131.0
54.90	125.0
55.90	530.0
57.00	967.0
58.10	126.0
60.10	367.0
61.00	1375.0
62.00	1830.0
63.00	1509.0
63.90	217.0
64.90	346.0
66.90	108.0
68.00	3166.0
69.00	3863.0
70.00	348.0
72.00	323.0
73.00	1822.0
74.00	5738.0
75.00	17256.0
76.00	1496.0
77.00	286.0
77.90	183.0
78.90	1093.0
79.80	357.0
80.90	1296.0
81.90	432.0
87.00	1791.0
87.90	1635.0
90.80	118.0
91.90	1101.0
93.00	1877.0
94.00	4255.0
95.00	35432.0
96.00	2719.0
96.90	105.0
103.90	175.0
105.80	250.0
115.80	120.0
116.90	247.0
118.10	146.0
118.90	243.0
127.90	165.0
128.80	112.0
129.90	155.0
141.00	320.0
142.90	481.0
147.90	128.0
154.70	157.0
171.80	332.0
173.00	448.0
174.00	31552.0
175.00	2351.0
175.90	30512.0
177.00	2038.0

Instrument :
MSVOA_V
ClientSampleId :
BFB234

m/z	Abundance
36.00	261.0
37.00	1479.0
37.90	1435.0
39.00	496.0
39.90	243.0
43.90	449.0
44.90	219.0
46.90	402.0
47.70	172.0
49.00	1207.0
50.00	5758.0
51.00	1915.0
51.90	134.0
54.90	103.0
55.90	468.0
57.00	895.0
58.10	123.0
60.00	361.0
61.00	1472.0
62.00	1704.0
63.00	1421.0
63.90	232.0
65.00	331.0
68.00	3115.0
69.00	3545.0
70.00	355.0
71.90	288.0
73.00	1656.0
74.00	5636.0
75.00	16480.0
76.00	1379.0
77.00	211.0
78.00	160.0
78.90	1174.0
79.80	359.0
80.90	1197.0
81.80	413.0
86.90	1561.0
87.90	1522.0
90.90	156.0
91.90	998.0
93.00	1687.0
94.00	3949.0
95.00	34224.0
96.00	2613.0
103.80	186.0
105.80	206.0
116.90	224.0
118.00	157.0
119.00	222.0
127.90	164.0
128.90	133.0
129.90	176.0
141.00	293.0
142.90	496.0
147.80	132.0
154.70	141.0
171.80	320.0
173.00	411.0
174.00	30528.0
175.00	2412.0
175.90	29472.0
177.00	1957.0

Instrument :
MSVOA_V
ClientSampleId :
BFB234