
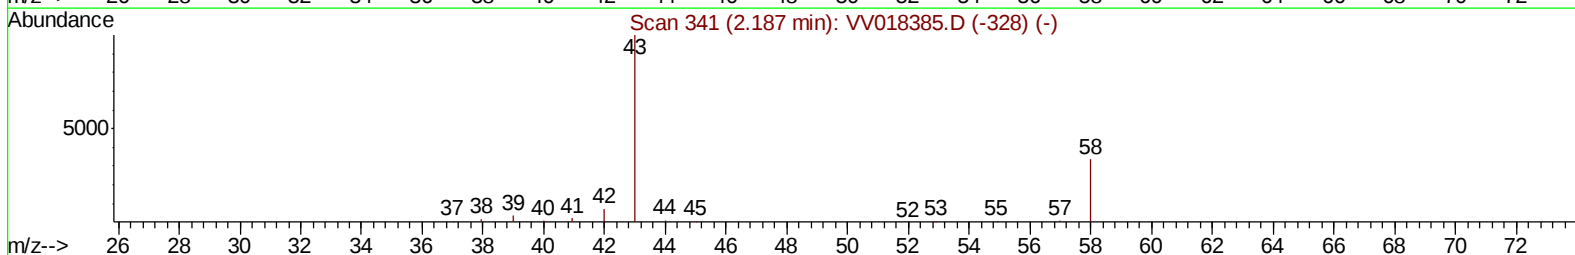
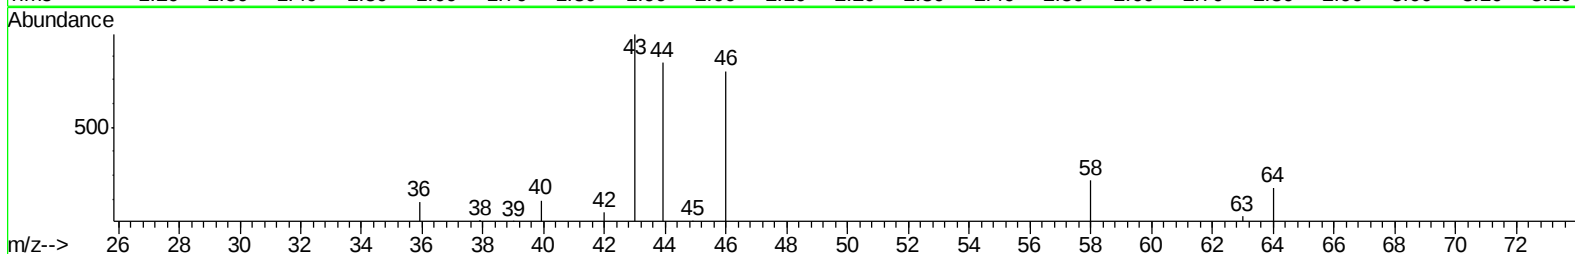


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV092220\
Data File : VV018393.D
Acq On : 22 Sep 2020 14:14
Operator : SY/MD
Sample : L4090-06RE
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 11 Sample Multiplier: 1

Quant Time: Sep 23 06:32:27 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Sep 23 05:49:41 2020
Response via : Initial Calibration

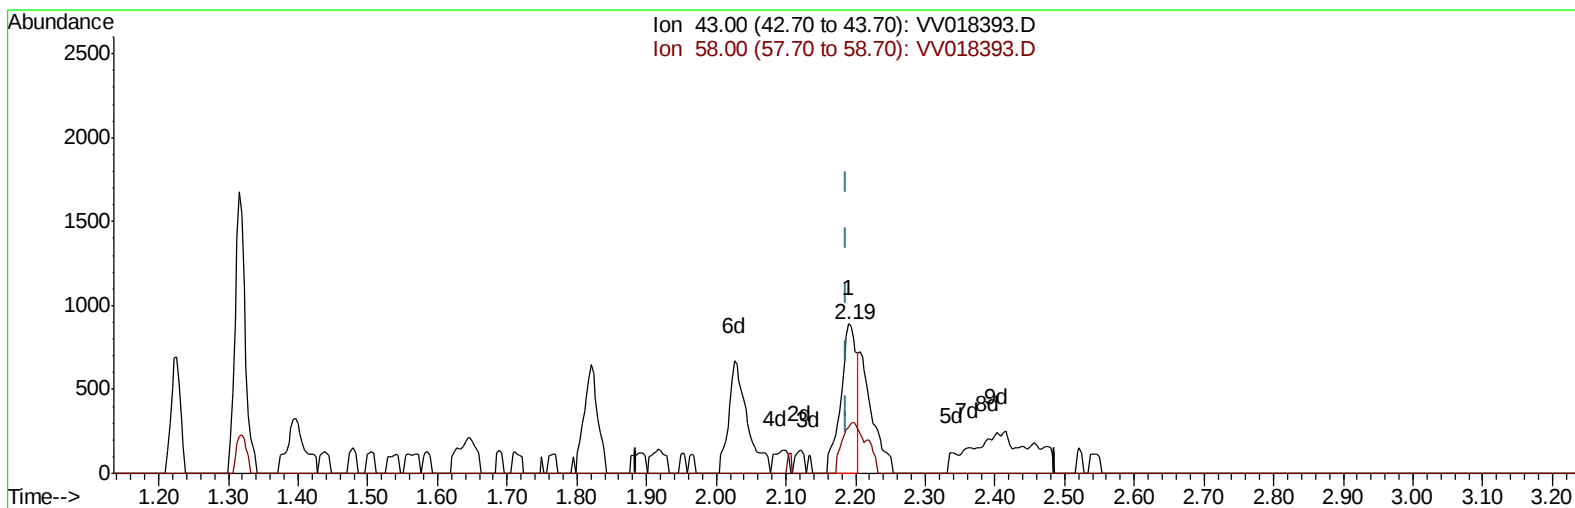

TIC: VV018393.D

(13) Acetone (T)

2.190min (+0.004) 2.75ug/L

response 1414

Ion	Exp%	Act%
43.00	100	100
58.00	33.70	41.09
0.00	0.00	0.00
0.00	0.00	0.00