
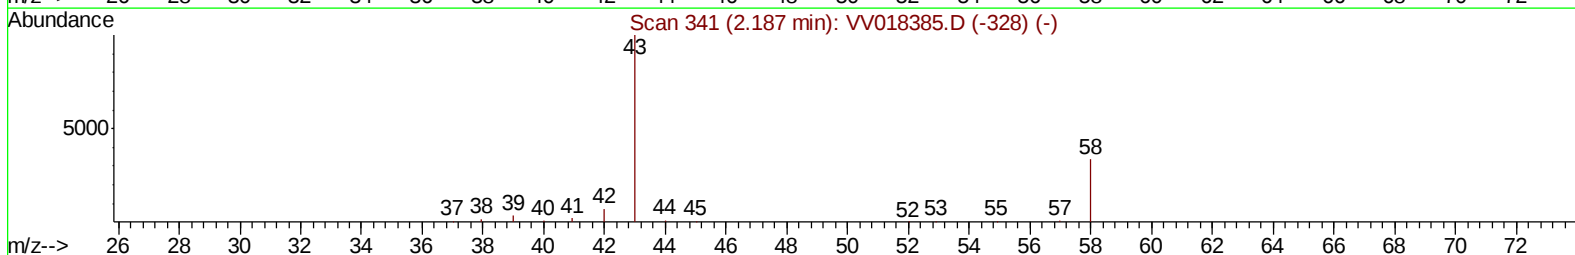
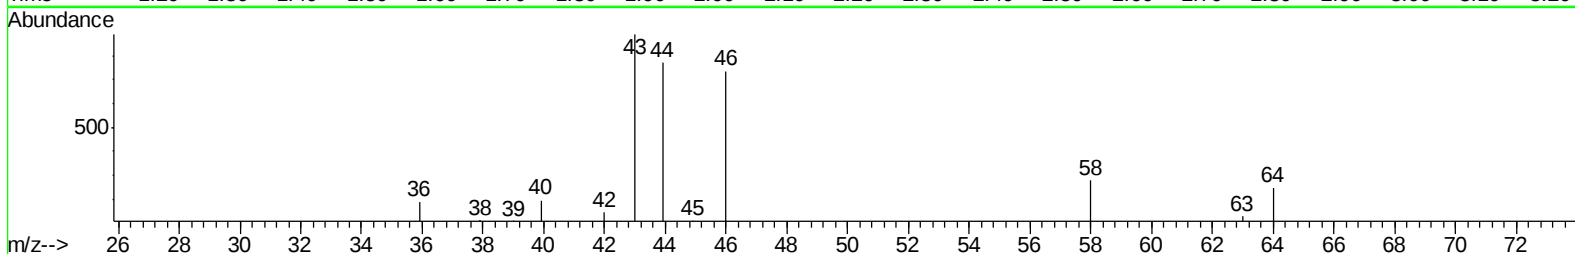


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092220\
 Data File : VV018393.D
 Acq On : 22 Sep 2020 14:14
 Operator : SY/MD
 Sample : L4090-06RE
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Quant Time: Sep 23 06:32:27 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Sep 23 05:49:41 2020
 Response via : Initial Calibration

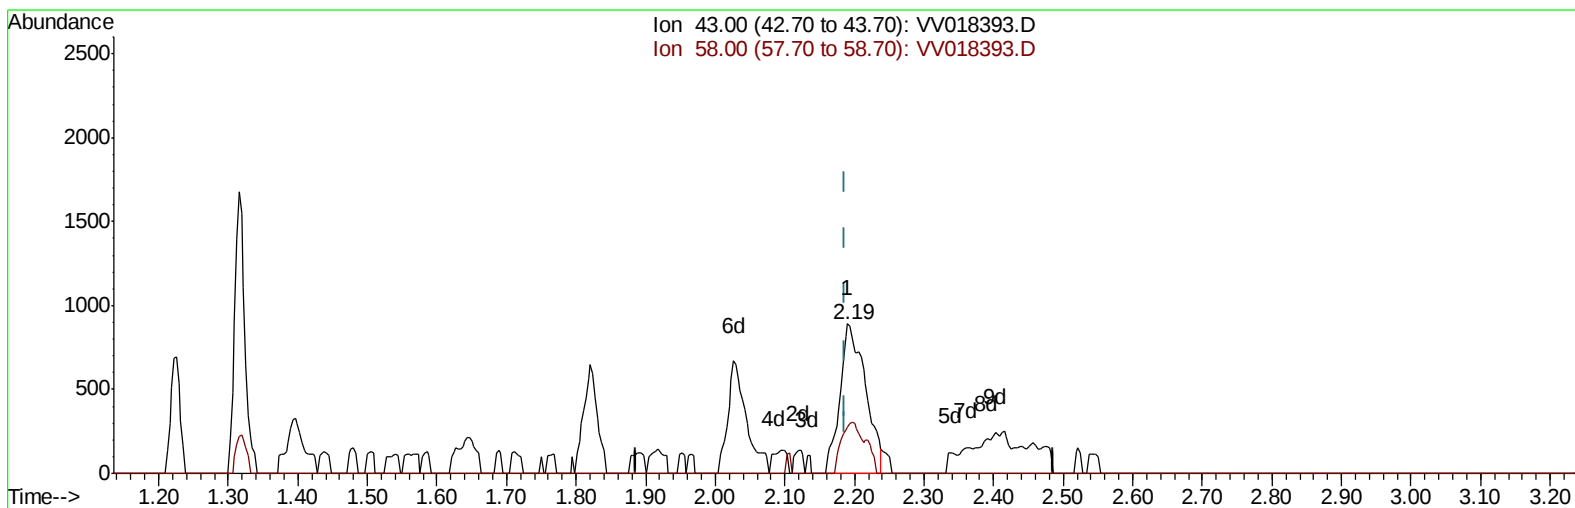

TIC: VV018393.D

(13) Acetone (T)

2.190min (+0.004) 4.44ug/L m

response 2285

Ion	Exp%	Act%
43.00	100	100
58.00	33.70	25.43
0.00	0.00	0.00
0.00	0.00	0.00