


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV092220\
 Data File : VV018384.D
 Acq On : 22 Sep 2020 09:29
 Operator : SY/MD
 Sample : BFB96
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB96

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Title : VOC Analysis
 Last Update : Wed Sep 23 05:49:41 2020

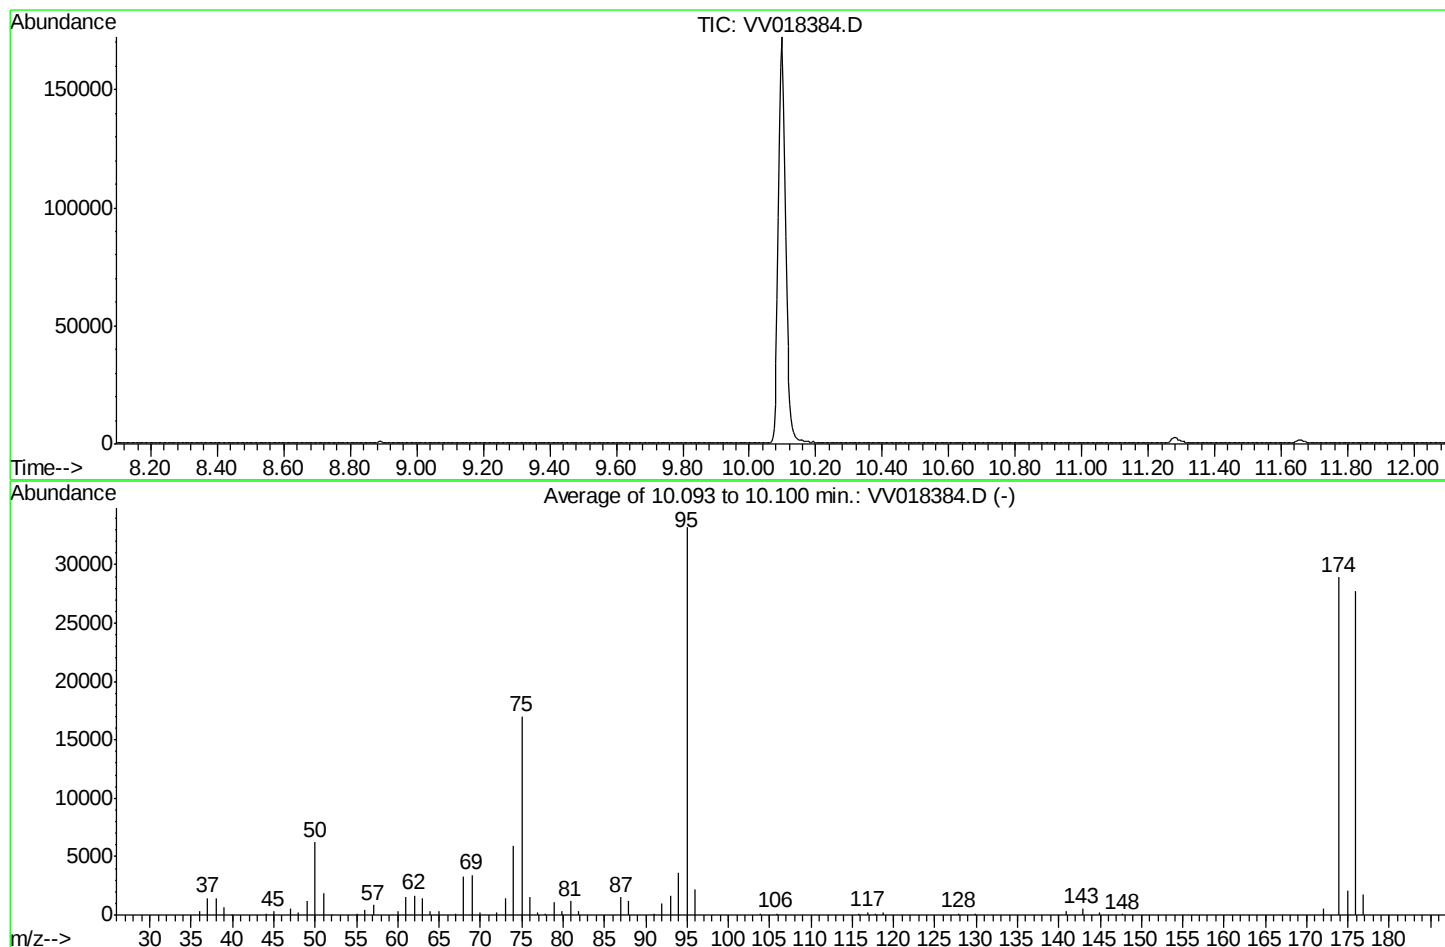

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2790

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	6227	PASS
75	95	30	80	51.2	16992	PASS
95	95	100	100	100.0	33208	PASS
96	95	5	9	6.6	2188	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	87.1	28912	PASS
175	174	5	9	7.3	2114	PASS
176	174	95	101	95.8	27704	PASS
177	176	5	9	6.2	1727	PASS

m/z	Abundance
35.90	291.0
37.00	1512.0
38.00	1408.0
39.00	621.0
40.00	230.0
44.00	416.0
45.00	283.0
47.00	497.0
47.90	250.0
49.00	1194.0
50.00	6167.0
51.00	1927.0
55.00	138.0
56.00	471.0
57.10	829.0
60.00	297.0
61.00	1596.0
62.00	1617.0
63.00	1343.0
63.90	292.0
64.90	351.0
68.00	3164.0
69.00	3336.0
69.90	229.0
71.90	167.0
73.00	1360.0
74.00	5667.0
75.00	16440.0
76.00	1598.0
77.10	176.0
77.90	135.0
78.90	1108.0
79.90	312.0
80.90	1112.0
81.80	345.0
87.00	1475.0
87.90	1281.0
90.90	113.0
92.00	977.0
93.00	1568.0
94.00	3524.0
95.00	31984.0
96.00	2116.0
104.00	126.0
105.90	154.0
116.90	260.0
117.80	129.0
118.80	255.0
127.90	143.0
129.80	140.0
140.90	333.0
142.80	461.0
144.90	207.0
171.90	484.0
173.90	26992.0
174.90	2094.0
175.90	25960.0
176.90	1731.0

Instrument :
MSVOA_V
ClientSampleId :
BFB96

m/z	Abundance
36.00	325.0
37.00	1526.0
38.00	1488.0
39.00	718.0
39.90	207.0
44.00	403.0
45.00	309.0
47.00	582.0
48.00	220.0
49.00	1261.0
50.00	6445.0
51.00	1961.0
51.90	116.0
55.00	124.0
56.00	473.0
57.00	867.0
60.00	354.0
61.00	1640.0
62.00	1715.0
63.00	1477.0
63.90	318.0
65.00	360.0
67.00	104.0
68.00	3383.0
69.00	3522.0
70.00	246.0
71.90	192.0
73.00	1461.0
74.00	6122.0
75.00	17608.0
76.00	1630.0
76.90	187.0
77.90	120.0
78.90	1114.0
79.90	347.0
80.90	1230.0
81.90	342.0
87.00	1559.0
87.90	1295.0
90.90	122.0
92.00	1024.0
93.00	1737.0
94.00	3779.0
95.00	34392.0
96.00	2244.0
103.90	130.0
105.80	168.0
115.80	106.0
116.90	272.0
117.80	123.0
118.80	270.0
127.90	162.0
129.90	139.0
140.90	360.0
142.90	509.0
145.00	222.0
147.70	105.0
171.90	501.0
173.90	30000.0
174.90	2172.0
175.90	28752.0
176.90	1766.0

Instrument :
MSVOA_V
ClientSampleId :
BFB96

m/z	Abundance
36.00	306.0
37.00	1401.0
38.00	1423.0
39.00	691.0
39.90	198.0
44.10	358.0
45.00	269.0
46.90	594.0
48.00	181.0
49.00	1248.0
50.00	6070.0
51.00	1844.0
55.90	455.0
57.00	857.0
60.00	367.0
61.00	1483.0
62.00	1707.0
63.00	1408.0
63.90	293.0
65.00	376.0
67.00	105.0
68.00	3244.0
69.00	3348.0
70.00	220.0
71.90	196.0
73.00	1334.0
74.00	5982.0
75.00	16928.0
76.00	1494.0
76.90	231.0
77.90	119.0
78.90	1037.0
79.90	363.0
80.90	1196.0
81.90	311.0
87.00	1488.0
87.90	1209.0
91.00	130.0
92.00	939.0
93.00	1652.0
94.00	3695.0
95.00	33248.0
96.00	2206.0
103.80	140.0
105.80	161.0
115.80	116.0
116.90	268.0
117.80	101.0
118.80	250.0
127.90	152.0
129.90	132.0
140.90	373.0
142.90	525.0
145.00	180.0
147.80	103.0
172.00	511.0
173.90	29744.0
174.90	2076.0
175.90	28400.0
176.90	1685.0

Instrument :
MSVOA_V
ClientSampleId :
BFB96

Scan 2790 (10.061 min): VV018384.D
BFB96

m/z	Abundance
39.90	187.0
44.00	265.0

Instrument :
MSVOA_V
ClientSampleId :
BFB96