




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092222\
 Data File : VV028083.D
 Acq On : 23 Sep 2022 01:09
 Operator : SY/MD
 Sample : N4621-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB8H3

Manual IntegrationsAPPROVED

Quant Time: Sep 23 04:54:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 23 04:38:54 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/23/2022
 Supervised By :Mahesh Dadoda 09/26/2022

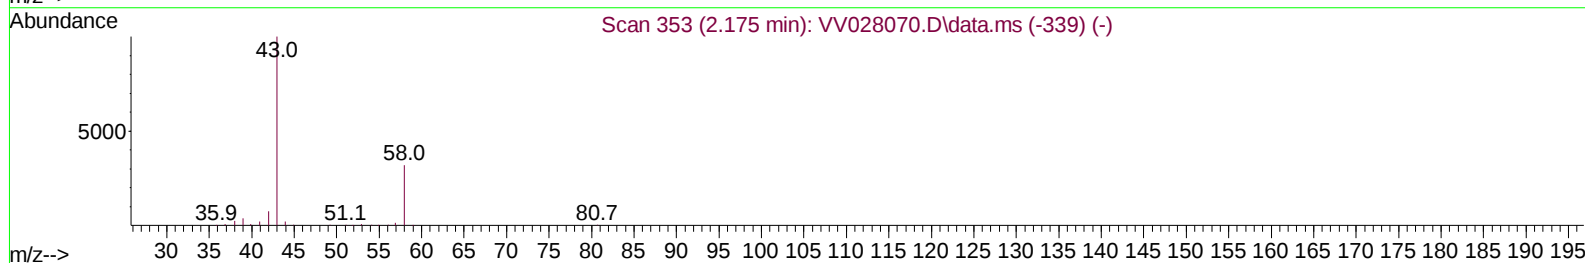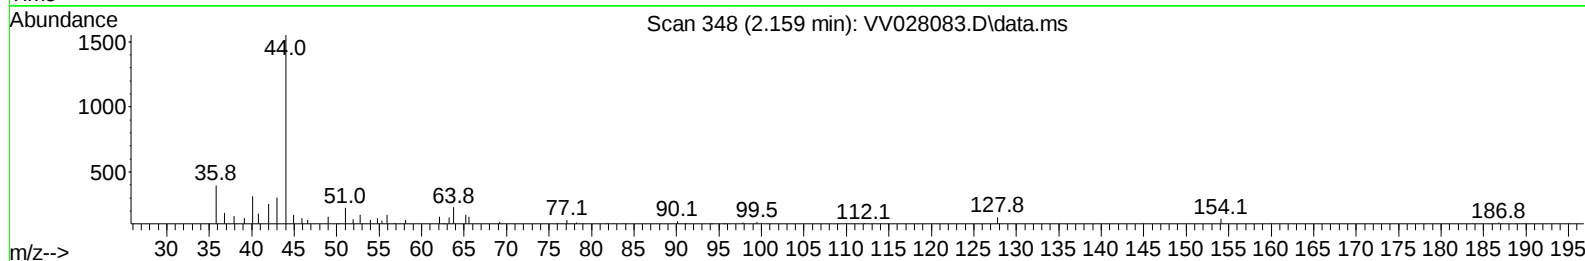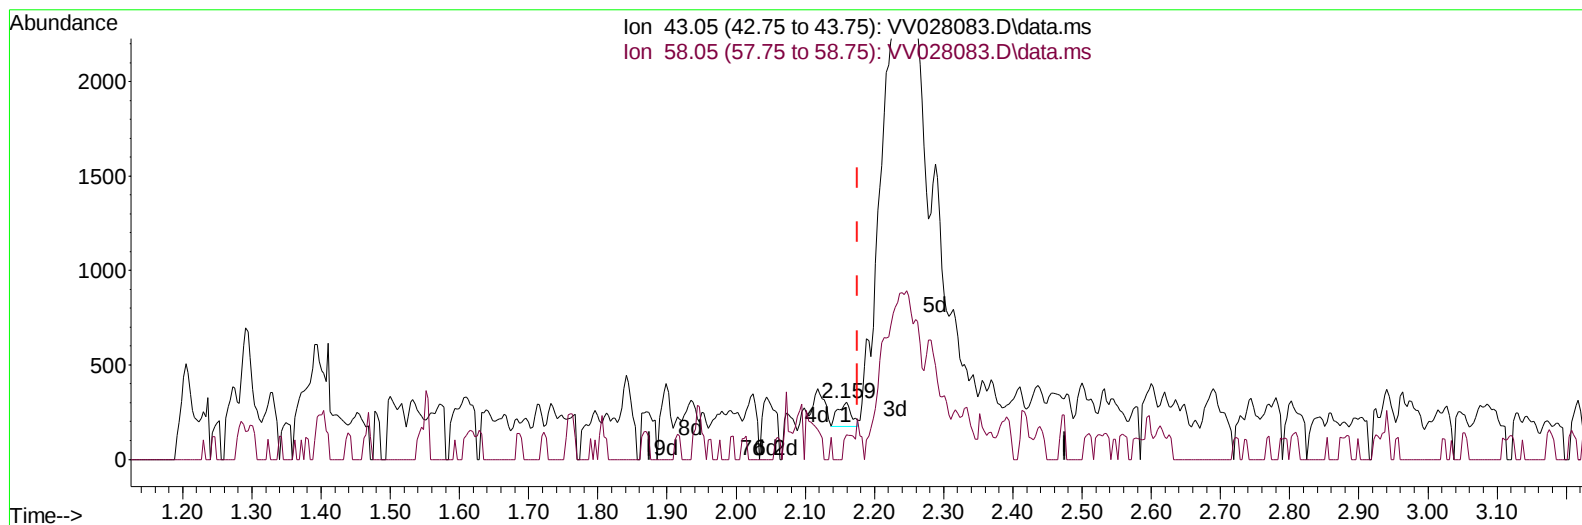

TIC: VV028083.D\data.ms

(13) Acetone (T)

2.159min (-0.016) 0.06 ug/L

response 180

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	32.80	65.00
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092222\
 Data File : VV028083.D
 Acq On : 23 Sep 2022 01:09
 Operator : SY/MD
 Sample : N4621-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB8H3

Manual IntegrationsAPPROVED

Quant Time: Sep 23 04:54:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 23 04:38:54 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/23/2022
 Supervised By :Mahesh Dadoda 09/26/2022

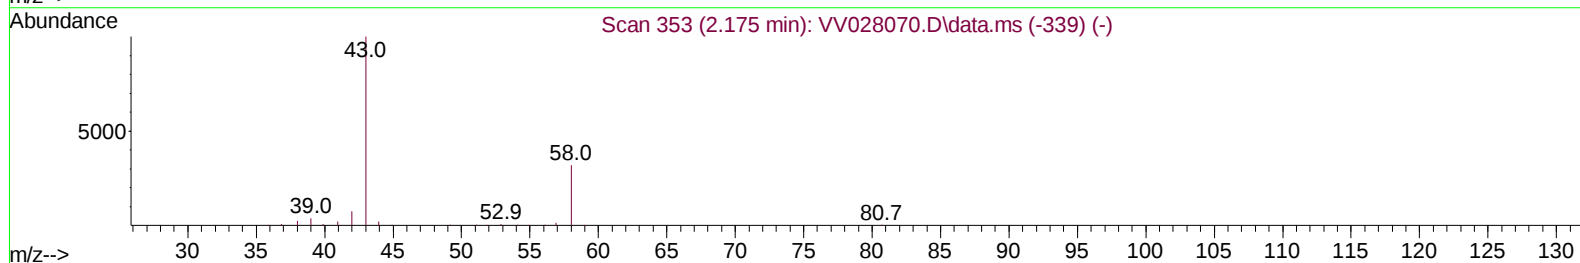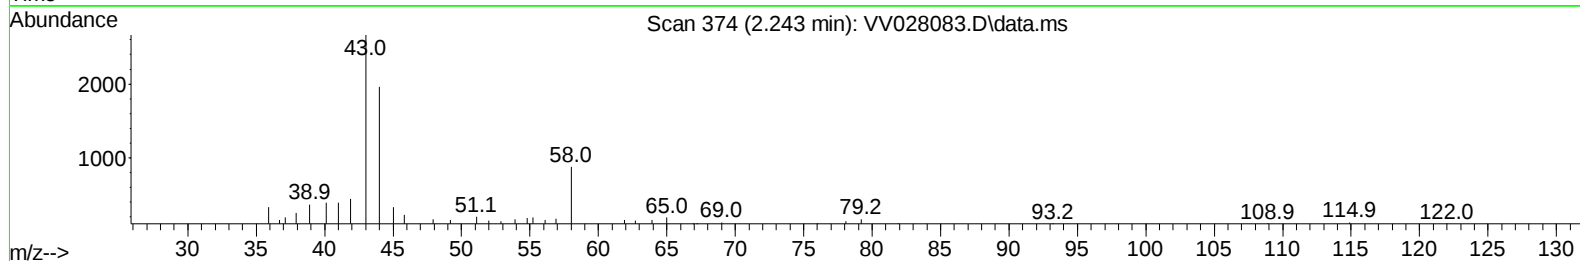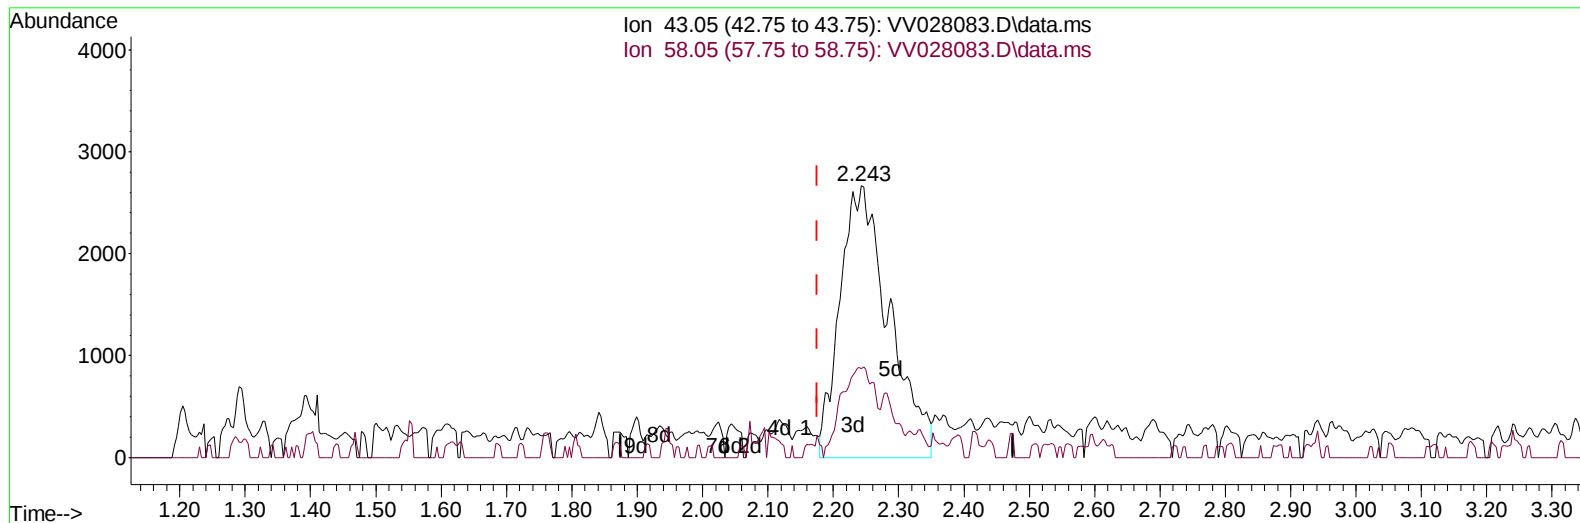

TIC: VV028083.D\data.ms

(13) Acetone (T)

2.243min (+ 0.068) 4.54 ug/L m

response 13920

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	32.80	0.84
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092222\
 Data File : VV028083.D
 Acq On : 23 Sep 2022 01:09
 Operator : SY/MD
 Sample : N4621-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB8H3

Manual IntegrationsAPPROVED

Quant Time: Sep 23 04:54:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 23 04:38:54 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/23/2022
 Supervised By :Mahesh Dadoda 09/26/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.603	114		227409	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.841	117		167879	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.243	152		77963	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.291	65		96075	4.075	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	81.600%	
7) Chloroethane-d5	1.552	69		76717	4.093	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	81.800%	
11) 1,1-Dichloroethene-d2	2.092	63		129619	3.170	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.400%	
20) 2-Butanone-d5	3.941	46		206597	51.906	ug/L	0.05
Spiked Amount	50.000	Range	40 - 130	Recovery	=	103.820%	
24) Chloroform-d	4.333	84		160775	4.274	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.400%	
26) 1,2-Dichloroethane-d4	5.024	65		83077	4.641	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.800%	
32) Benzene-d6	5.031	84		332876	6.047	ug/L	-0.01
Spiked Amount	5.000	Range	70 - 125	Recovery	=	121.000%	
36) 1,2-Dichloropropane-d6	6.056	67		99381	5.791	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	115.800%	
41) Toluene-d8	7.294	98		237732	4.771	ug/L	-0.02
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.400%	
43) trans-1,3-Dichloroprop...	7.609	79		29245	4.718	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	94.400%	
46) 2-Hexanone-d5	8.101	63		116565	45.055	ug/L	0.02
Spiked Amount	50.000	Range	45 - 130	Recovery	=	90.100%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84		55918	4.767	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.400%	
66) 1,2-Dichlorobenzene-d4	11.619	152		82035	5.365	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.200%	
Target Compounds							
13) Acetone	2.243	43		13920m	4.540	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092222\
Data File : VV028083.D
Acq On : 23 Sep 2022 01:09
Operator : SY/MD
Sample : N4621-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 3

Instrument :
MSVOA_V
ClientSampleId :
CB8H3

Manual IntegrationsAPPROVED

Quant Time: Sep 23 04:54:01 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 23 04:38:54 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 09/23/2022
Supervised By :Mahesh Dadoda 09/26/2022

