

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092222\
 Data File : VV028068.D
 Acq On : 22 Sep 2022 18:11
 Operator : SY/MD
 Sample : VIBLK291
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK291

Quant Time: Sep 23 04:24:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 23 04:15:29 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	198175	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	192347	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	86147	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	92609	4.508	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	90.200%
7) Chloroethane-d5	1.561	69	74735	4.575	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	91.600%
11) 1,1-Dichloroethene-d2	2.098	63	122411	3.435	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.800%
20) 2-Butanone-d5	3.886	46	153821	44.347	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	88.700%
24) Chloroform-d	4.339	84	152271	4.645	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.800%
26) 1,2-Dichloroethane-d4	5.027	65	74929	4.803	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.000%
32) Benzene-d6	5.043	84	303955	4.819	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.400%
36) 1,2-Dichloropropane-d6	6.066	67	92367	4.698	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.000%
41) Toluene-d8	7.310	98	242840	4.254	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.000%
43) trans-1,3-Dichloroprop...	7.622	79	32590	4.589	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.800%
46) 2-Hexanone-d5	8.085	63	139618	47.101	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	94.200%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	62107	4.621	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.400%
66) 1,2-Dichlorobenzene-d4	11.622	152	86473	5.118	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.400%
Target Compounds						Qvalue
16) Methylene chloride	2.500	84	8597	0.562	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092222\
Data File : VV028068.D
Acq On : 22 Sep 2022 18:11
Operator : SY/MD
Sample : VIBLK291
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK291


Quant Time: Sep 23 04:24:17 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 23 04:15:29 2022
Response via : Initial Calibration

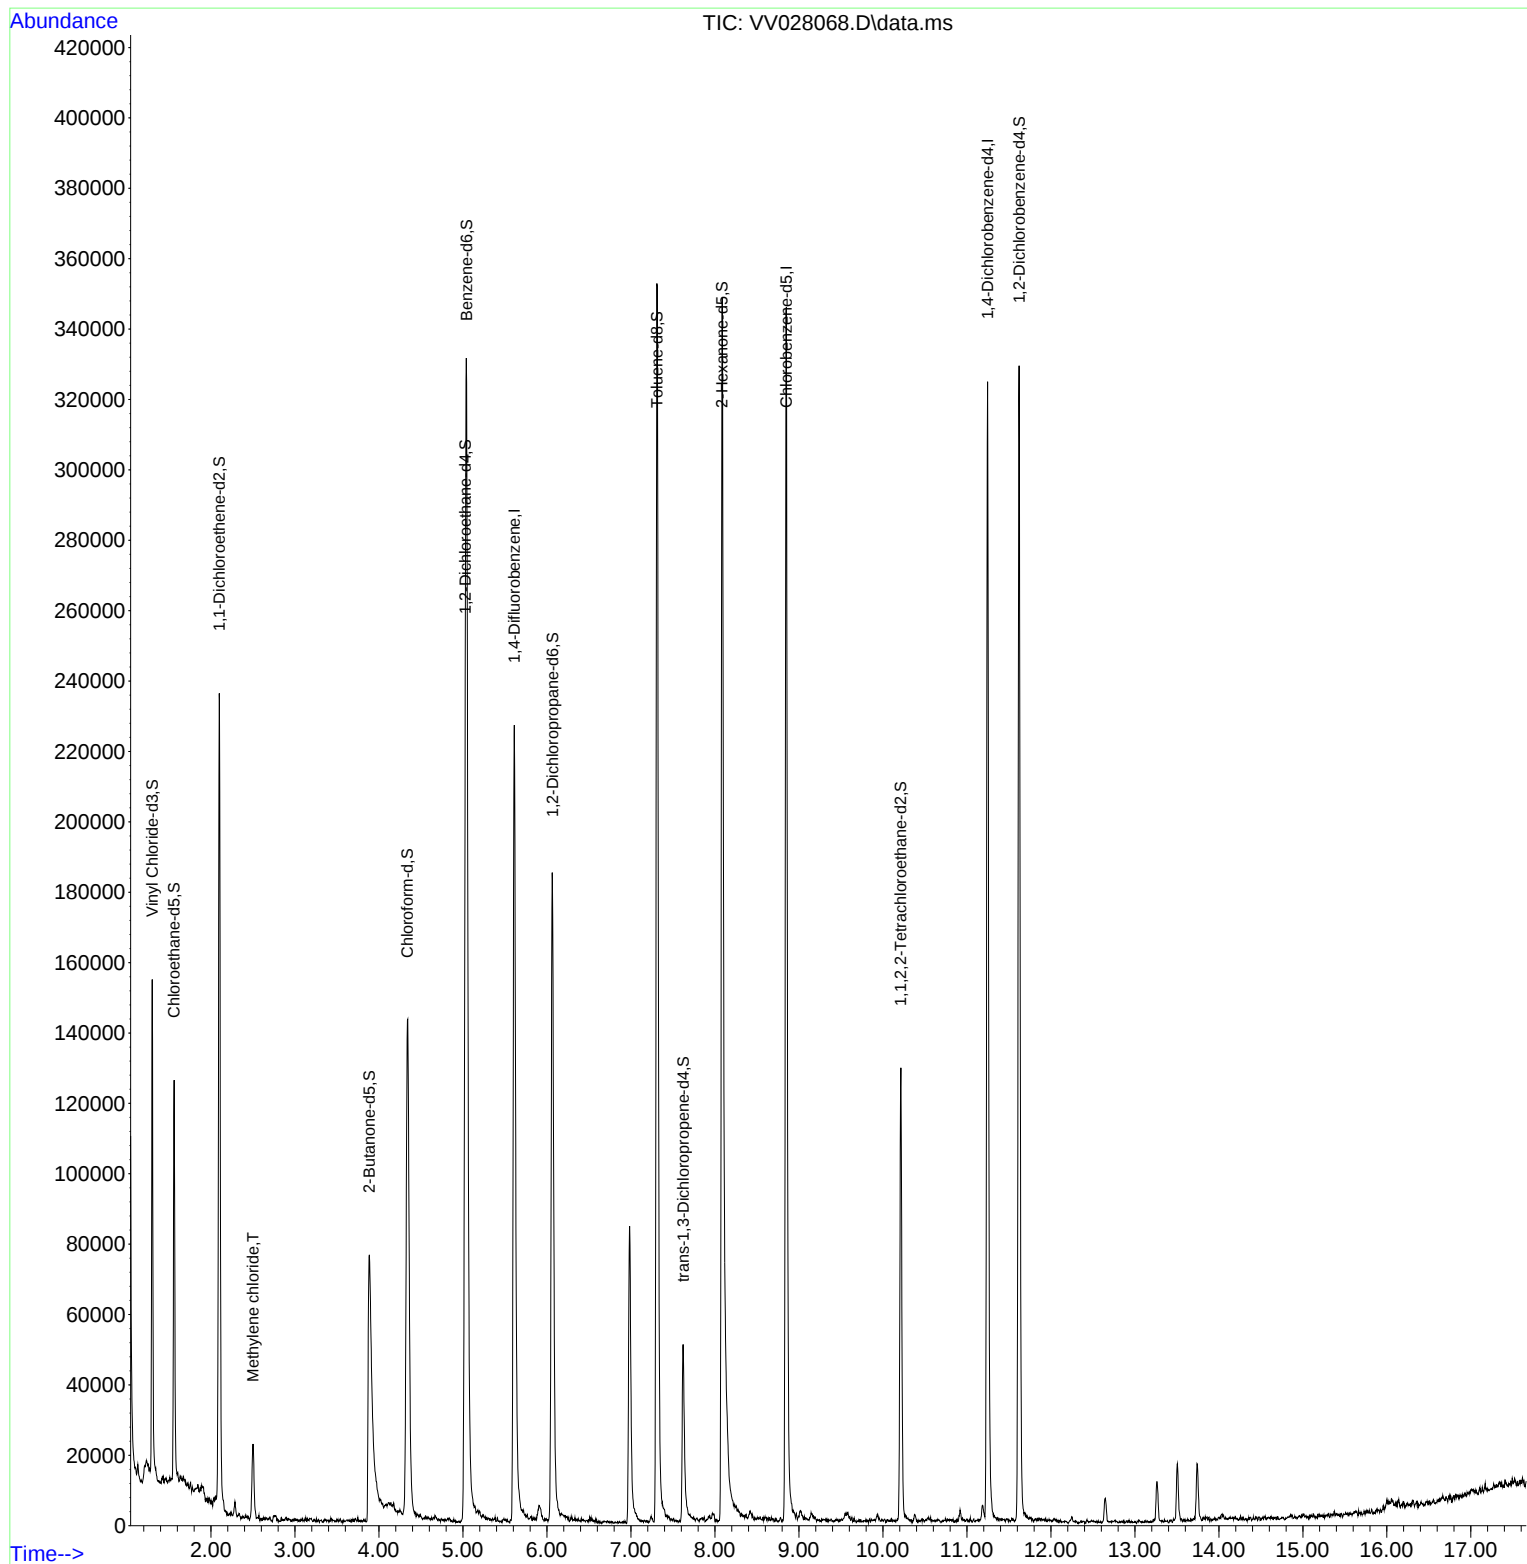

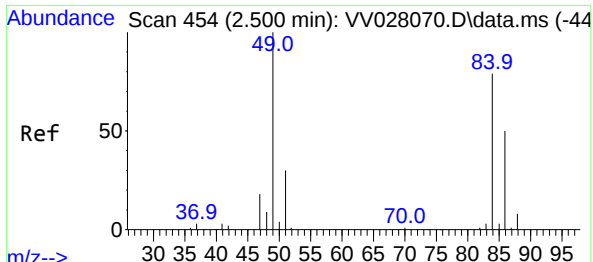

#16
Methylene chloride
Concen: 0.562 ug/L
RT: 2.500 min Scan# 4
Delta R.T. -0.000 min
Lab File: VV028068.D
Acq: 22 Sep 2022 18:11

Instrument :
MSVOA_V
ClientSampleId :
VIBLK291

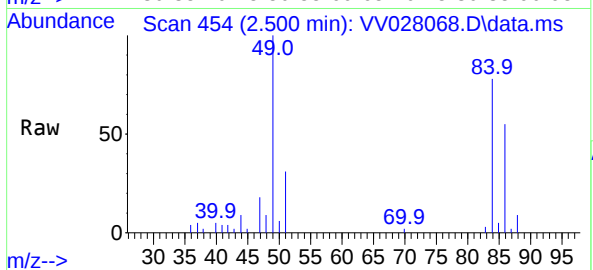

Tgt Ion: 84 Resp: 8597
Ion Ratio Lower Upper
84 100
86 71.0 46.8 86.8
49 128.8 87.5 162.5

