

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092222\
 Data File : VV028078.D
 Acq On : 22 Sep 2022 23:07
 Operator : SY/MD
 Sample : N4652-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Sep 23 04:52:59 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 23 04:38:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	205151	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	211203	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	96767	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	95030	4.468	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	89.400%
7) Chloroethane-d5	1.561	69	77722	4.596	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	92.000%
11) 1,1-Dichloroethene-d2	2.101	63	124089	3.364	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.200%
20) 2-Butanone-d5	3.873	46	161182	44.889	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	89.780%
24) Chloroform-d	4.343	84	153738	4.530	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.600%
26) 1,2-Dichloroethane-d4	5.027	65	73536	4.553	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.000%
32) Benzene-d6	5.043	84	290652	4.197	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.000%
36) 1,2-Dichloropropane-d6	6.066	67	93412	4.327	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	86.600%
41) Toluene-d8	7.314	98	241725	3.856	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	77.200%
43) trans-1,3-Dichloroprop...	7.619	79	29815	3.823	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	76.400%
46) 2-Hexanone-d5	8.085	63	122558	37.654	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	75.300%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	61514	4.168	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	83.400%
66) 1,2-Dichlorobenzene-d4	11.622	152	88138	4.644	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	92.800%
Target Compounds						Qvalue
16) Methylene chloride	2.503	84	9101	0.575	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092222\
Data File : VV028078.D
Acq On : 22 Sep 2022 23:07
Operator : SY/MD
Sample : N4652-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Sep 23 04:52:59 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 23 04:38:54 2022
Response via : Initial Calibration

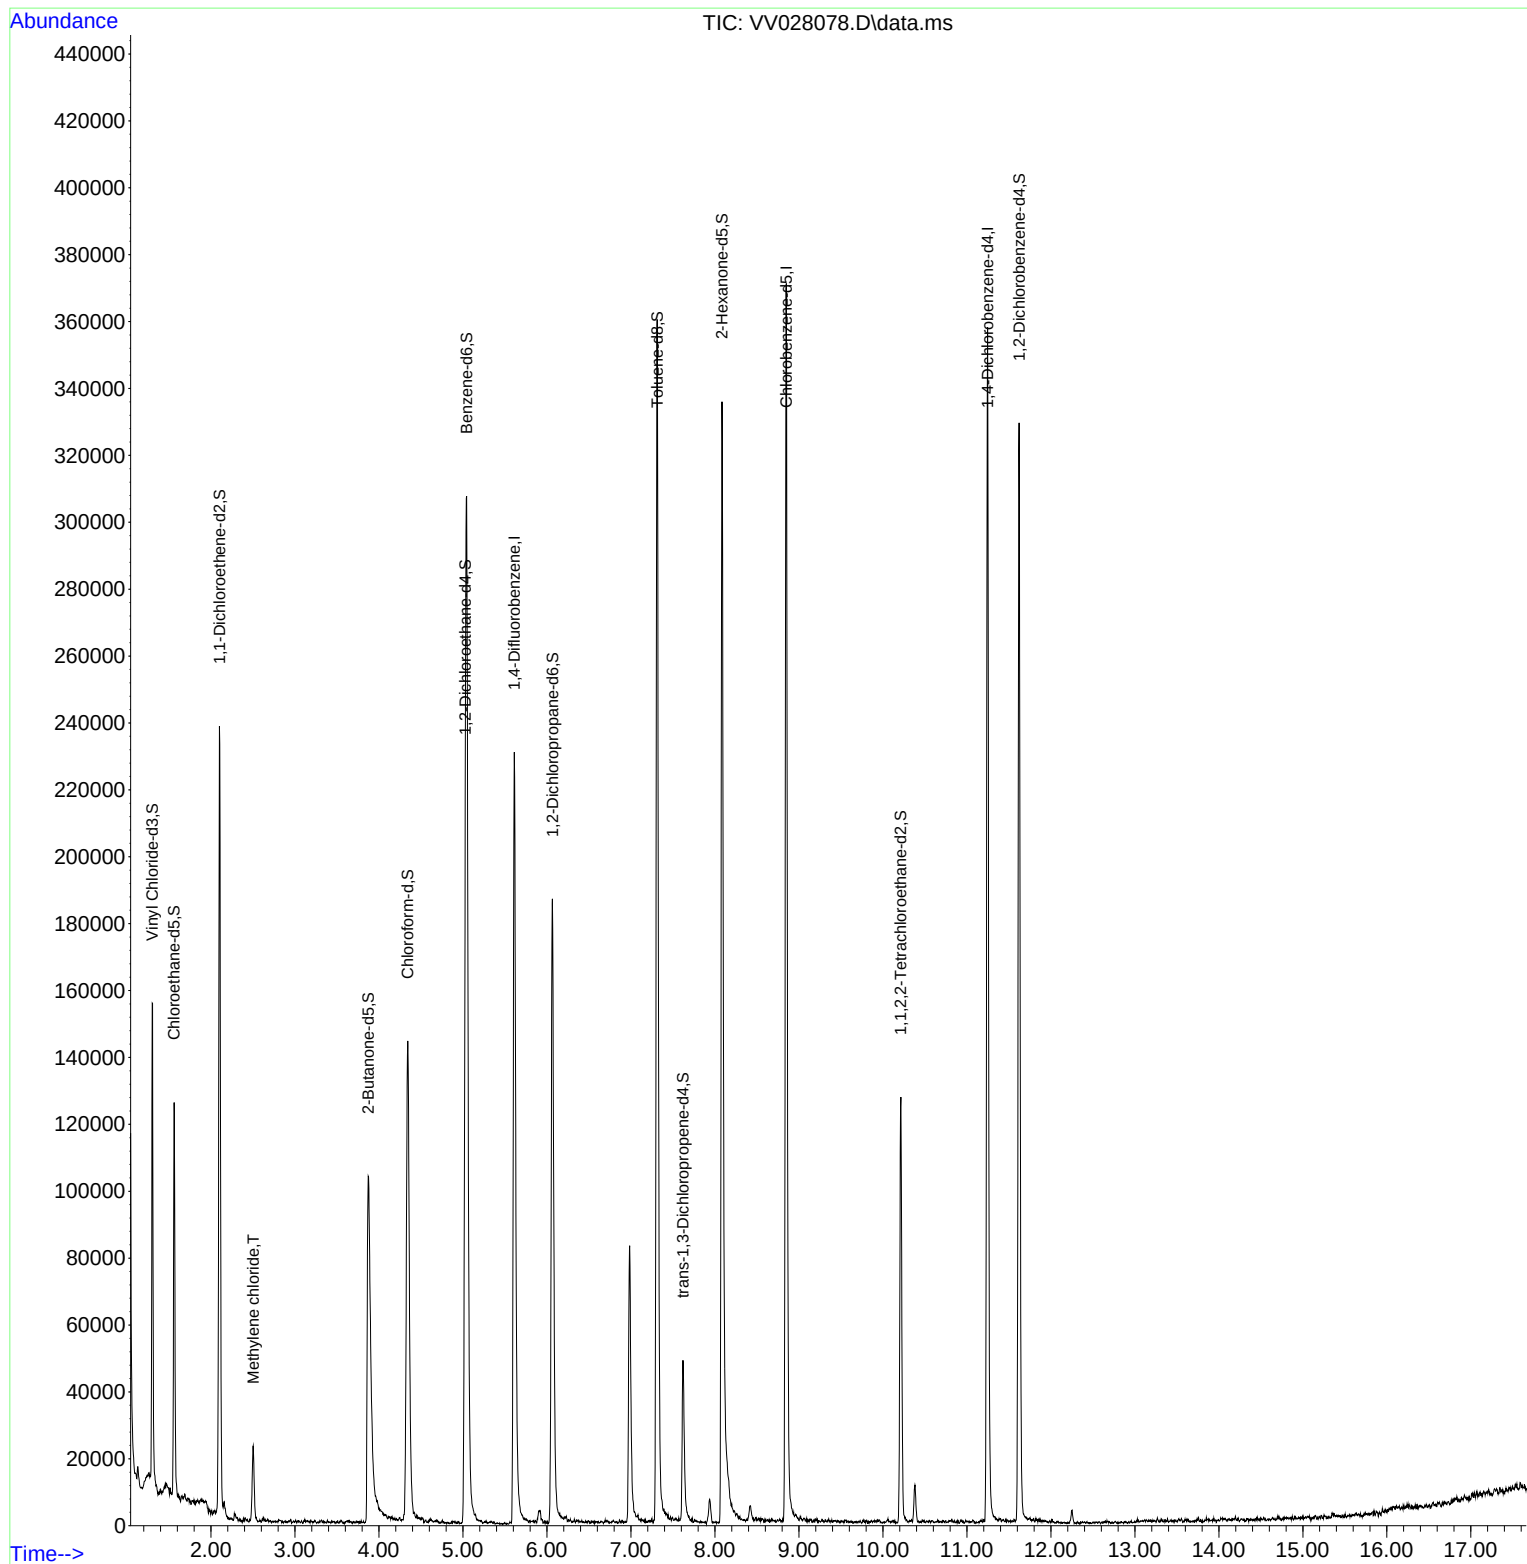

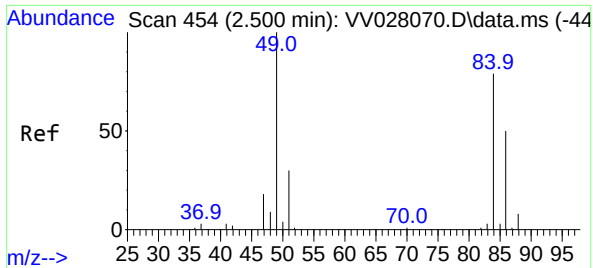

#16
Methylene chloride
Concen: 0.575 ug/L
RT: 2.503 min Scan# 4
Delta R.T. 0.003 min
Lab File: VV028078.D
Acq: 22 Sep 2022 23:07

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Tgt Ion:	84	Resp:	9101
Ion	Ratio	Lower	Upper
84	100		
86	60.2	46.8	86.8
49	116.5	87.5	162.5

