

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092222\
 Data File : VV028079.D
 Acq On : 22 Sep 2022 23:31
 Operator : SY/MD
 Sample : N4621-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB8G4

Quant Time: Sep 23 04:53:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 23 04:38:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	184195	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	182231	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	86532	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	92533	4.846	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	97.000%
7) Chloroethane-d5	1.561	69	77404	5.098	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	102.000%
11) 1,1-Dichloroethene-d2	2.101	63	126105	3.807	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	76.200%
20) 2-Butanone-d5	3.873	46	144753	44.900	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	89.800%
24) Chloroform-d	4.343	84	144579	4.745	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.800%
26) 1,2-Dichloroethane-d4	5.027	65	68058	4.694	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.800%
32) Benzene-d6	5.043	84	284976	4.769	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.400%
36) 1,2-Dichloropropane-d6	6.063	67	86036	4.619	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	92.400%
41) Toluene-d8	7.314	98	236209	4.367	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.400%
43) trans-1,3-Dichloroprop...	7.622	79	29971	4.454	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.000%
46) 2-Hexanone-d5	8.085	63	115898	41.269	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	82.540%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	55060	4.324	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.400%
66) 1,2-Dichlorobenzene-d4	11.622	152	87468	5.153	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.000%
Target Compounds						Qvalue
3) Chloromethane	1.237	50	9734	0.534	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092222\
Data File : VV028079.D
Acq On : 22 Sep 2022 23:31
Operator : SY/MD
Sample : N4621-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB8G4

Quant Time: Sep 23 04:53:09 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 23 04:38:54 2022
Response via : Initial Calibration

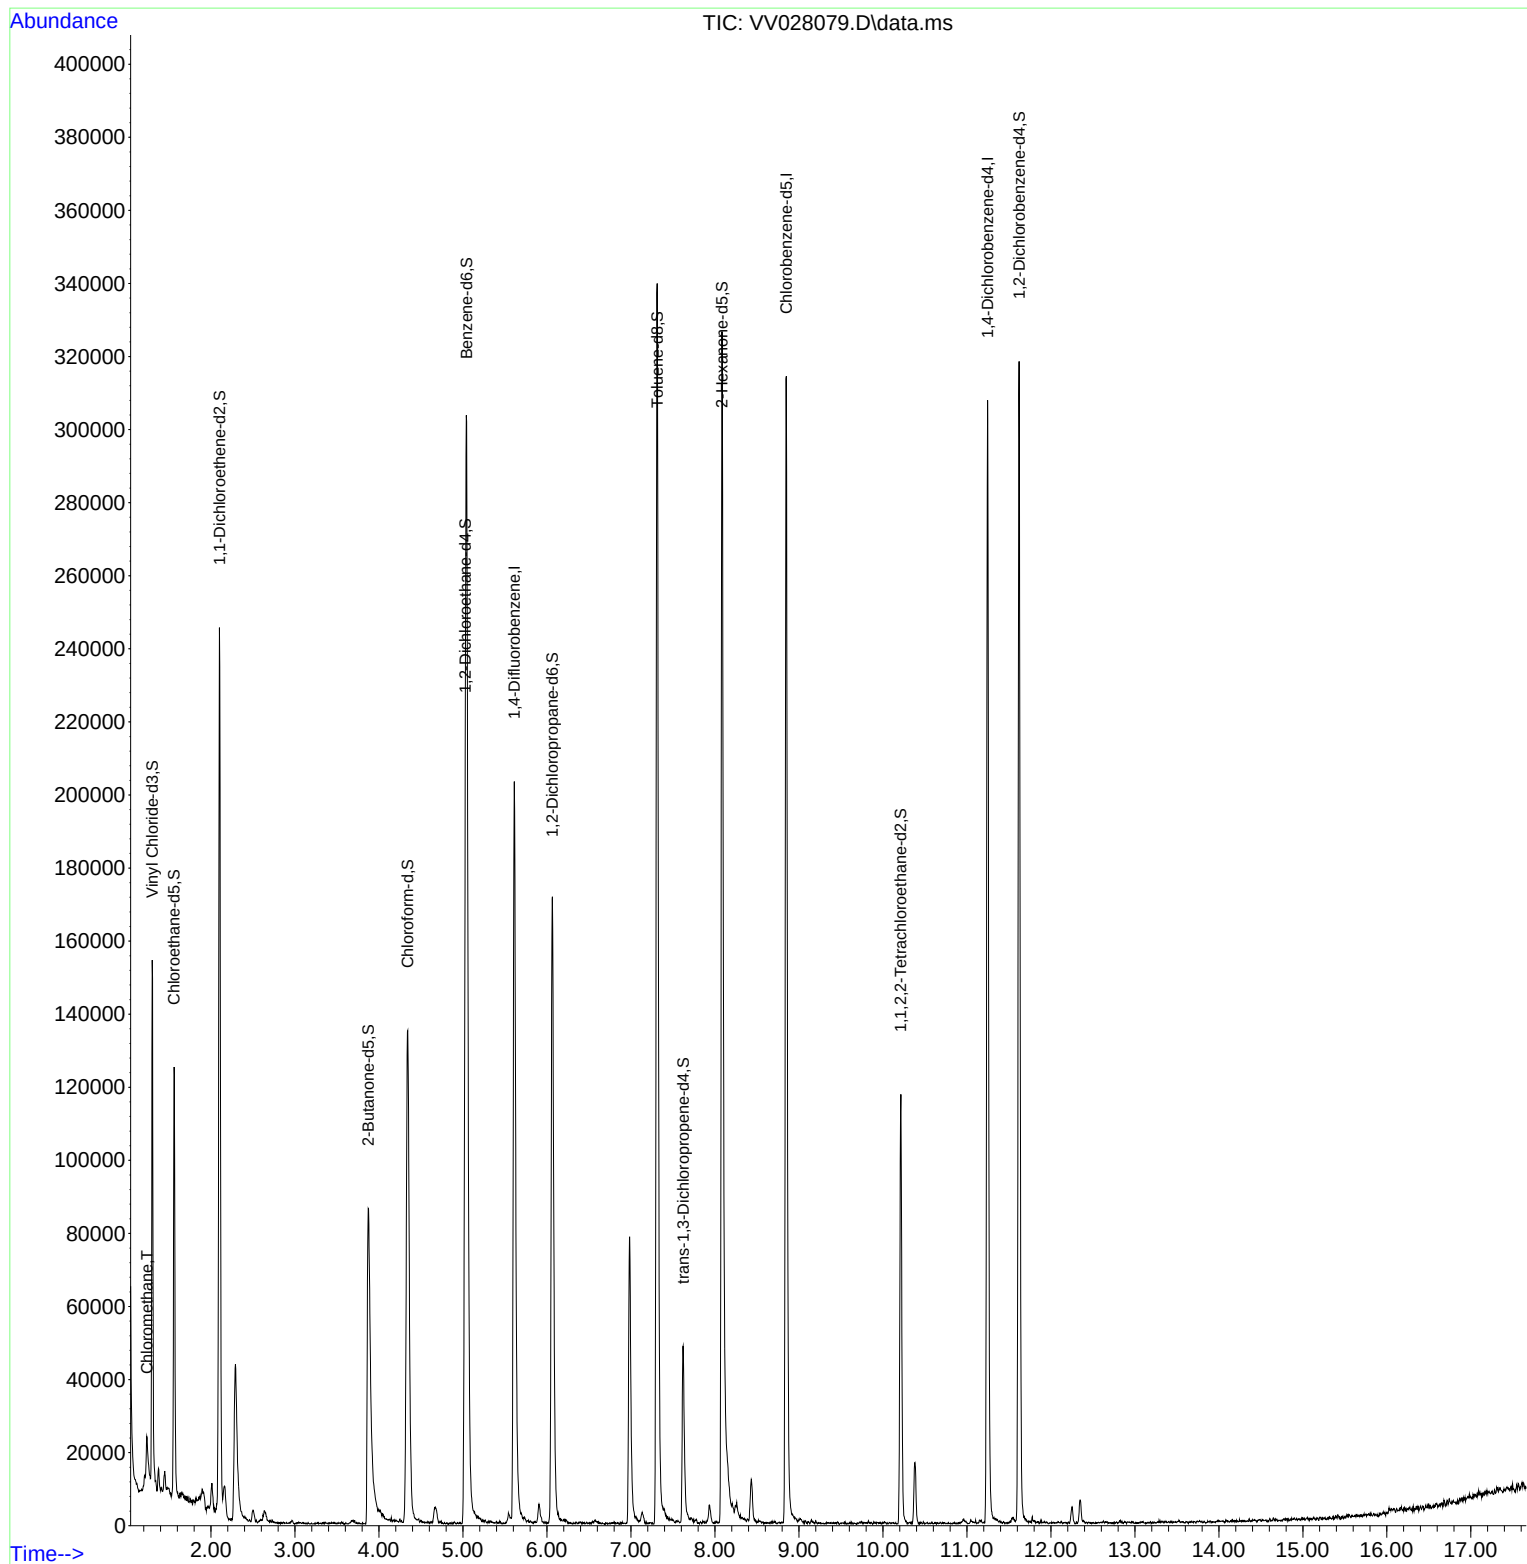

Abundance Scan 61 (1.236 min): VV028070.D\data.ms (-52)

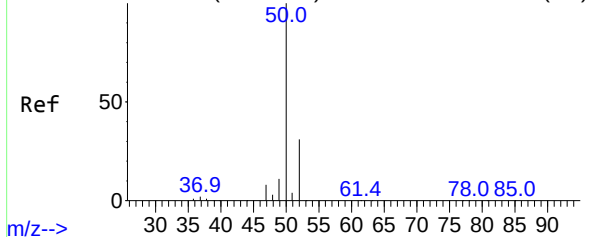


#3
Chloromethane
Concen: 0.534 ug/L
RT: 1.237 min Scan# 61
Delta R.T. 0.000 min
Lab File: VV028079.D
Acq: 22 Sep 2022 23:31

Instrument :
MSVOA_V
ClientSampleId :
CB8G4

Tgt Ion: 50 Resp: 9734
Ion Ratio Lower Upper
50 100
52 33.2 24.4 45.2

Abundance Scan 61 (1.237 min): VV028079.D\data.ms

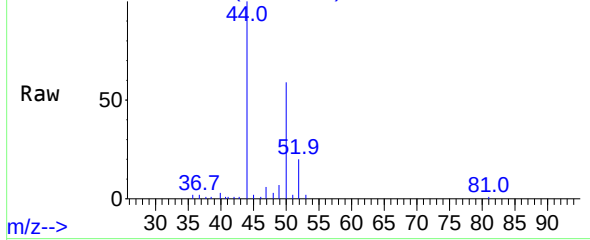

Abundance Scan 61 (1.237 min): VV028079.D\data.ms (-1) (

