

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092222\
 Data File : VV028081.D
 Acq On : 23 Sep 2022 00:20
 Operator : SY/MD
 Sample : N4621-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB8G9

Quant Time: Sep 23 04:53:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 23 04:38:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	182527	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	183801	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	94557	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	93132	4.922	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	98.400%	
7) Chloroethane-d5	1.561	69	75851	5.042	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	100.800%	
11) 1,1-Dichloroethene-d2	2.101	63	126736	3.861	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	77.200%	
20) 2-Butanone-d5	3.889	46	126379	39.559	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	79.120%	
24) Chloroform-d	4.343	84	148692	4.924	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	98.400%	
26) 1,2-Dichloroethane-d4	5.027	65	74386	5.177	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	103.600%	
32) Benzene-d6	5.043	84	306957	5.093	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	101.800%	
36) 1,2-Dichloropropane-d6	6.063	67	93964	5.001	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	100.000%	
41) Toluene-d8	7.313	98	257627	4.723	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	94.400%	
43) trans-1,3-Dichloroprop...	7.622	79	32393	4.773	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	95.400%	
46) 2-Hexanone-d5	8.085	63	128611	45.405	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	90.800%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	64928	5.056	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	101.200%	
66) 1,2-Dichlorobenzene-d4	11.622	152	104302	5.624	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	112.400%	
Target Compounds						
13) Acetone	2.172	43	12946	5.261	ug/L	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092222\
Data File : VV028081.D
Acq On : 23 Sep 2022 00:20
Operator : SY/MD
Sample : N4621-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB8G9

Quant Time: Sep 23 04:53:35 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 23 04:38:54 2022
Response via : Initial Calibration

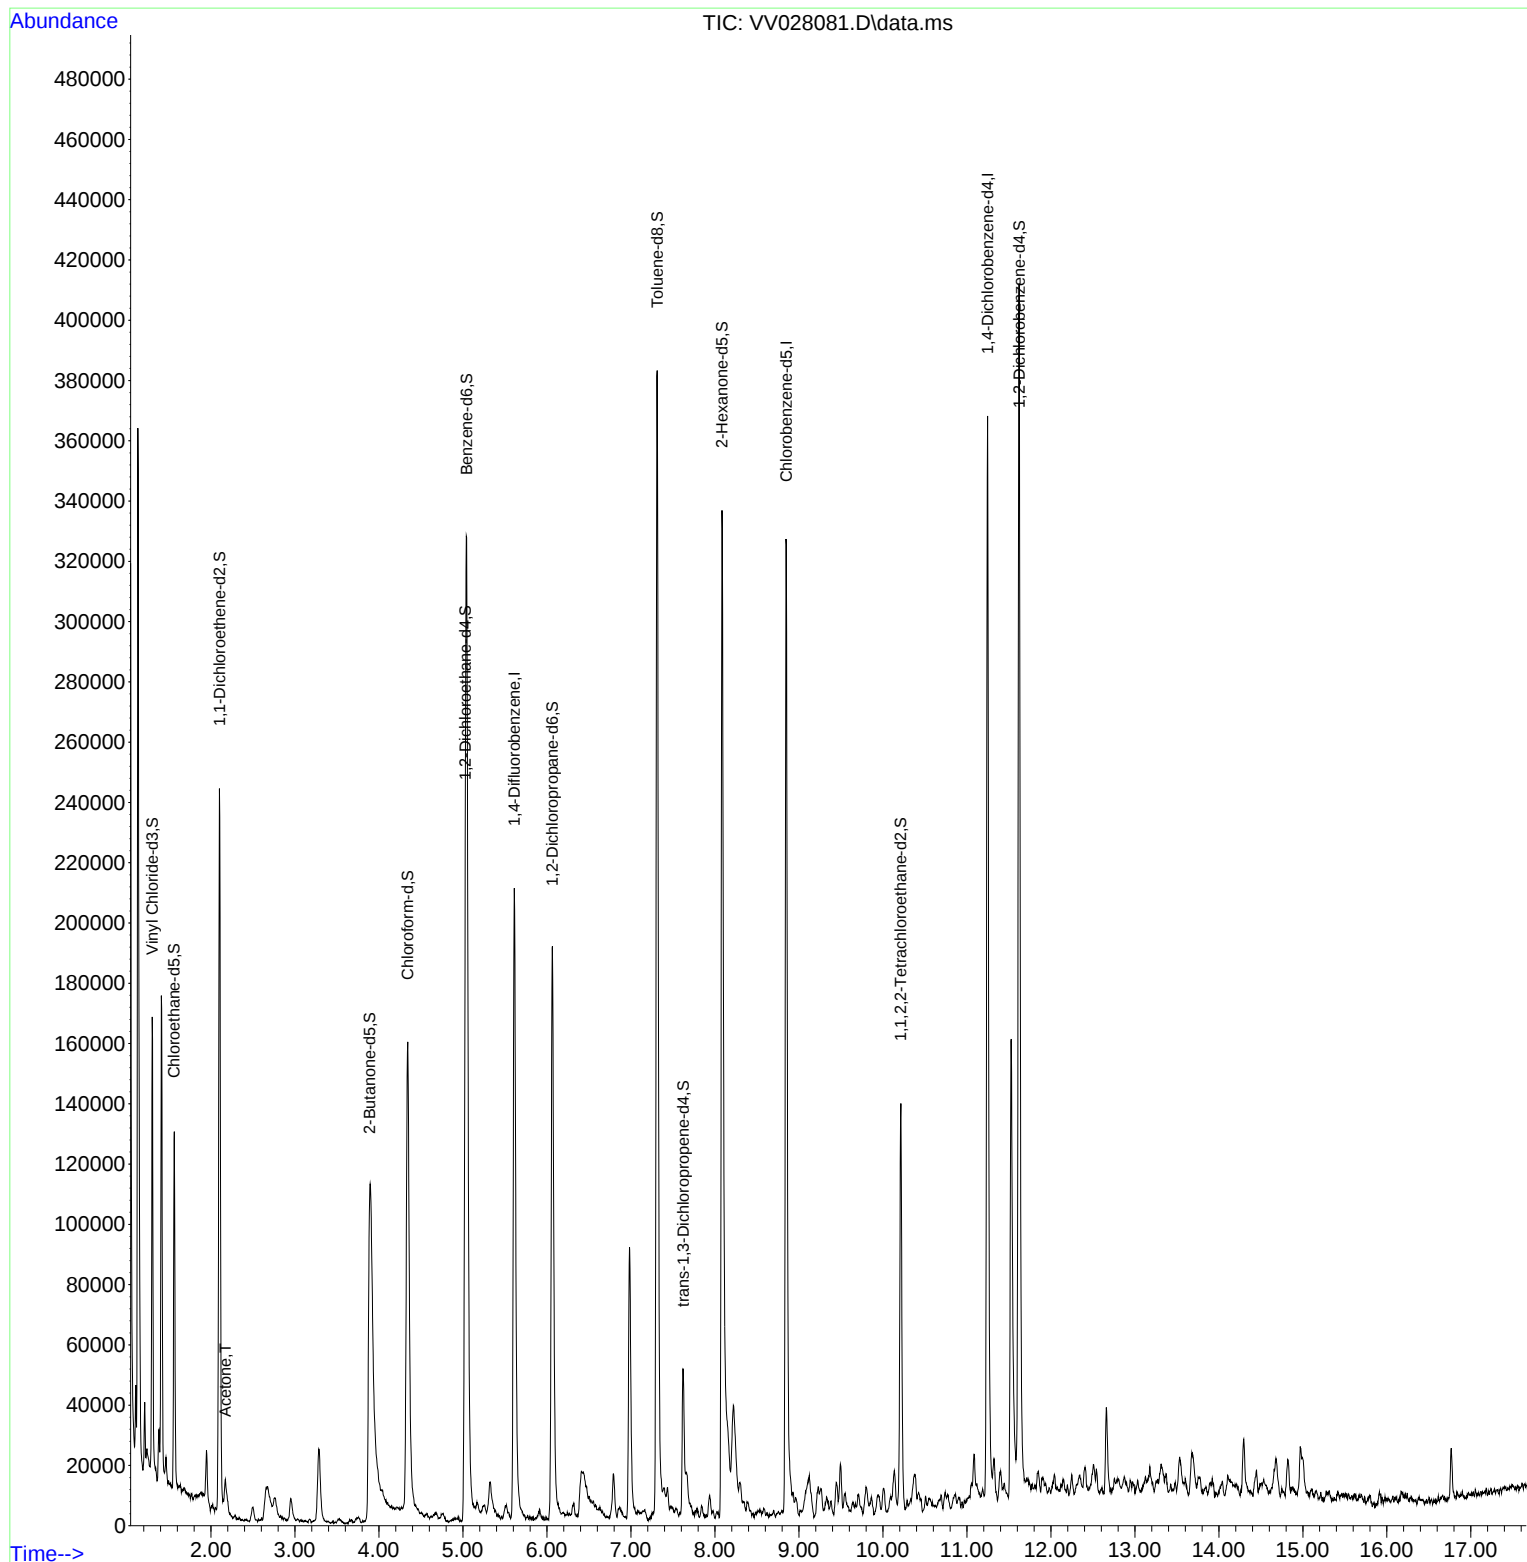

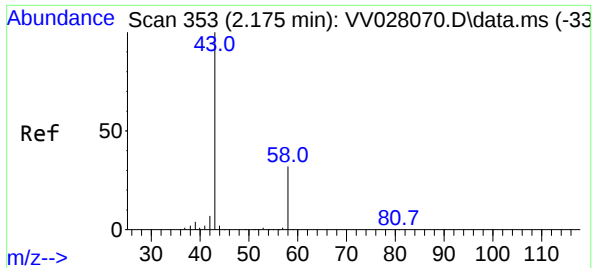

#13
Acetone
Concen: 5.261 ug/L
RT: 2.172 min Scan# 31
Delta R.T. -0.003 min
Lab File: VV028081.D
Acq: 23 Sep 2022 00:20

Instrument :
MSVOA_V
ClientSampleId :
CB8G9

Tgt Ion: 43 Resp: 12946
Ion Ratio Lower Upper
43 100
58 35.5 0.0 65.6

