

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092222\
 Data File : VV028083.D
 Acq On : 23 Sep 2022 01:09
 Operator : SY/MD
 Sample : N4621-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB8H3

Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 09/23/2022
 Supervised By :Mahesh Dadoda 09/26/2022

Quant Time: Sep 23 04:54:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 23 04:38:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.603	114	227409	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.841	117	167879	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.243	152	77963	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.291	65	96075	4.075	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	81.600%	
7) Chloroethane-d5	1.552	69	76717	4.093	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	81.800%	
11) 1,1-Dichloroethene-d2	2.092	63	129619	3.170	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	63.400%	
20) 2-Butanone-d5	3.941	46	206597	51.906	ug/L	0.05
Spiked Amount	50.000	Range 40 - 130	Recovery	=	103.820%	
24) Chloroform-d	4.333	84	160775	4.274	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	85.400%	
26) 1,2-Dichloroethane-d4	5.024	65	83077	4.641	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	92.800%	
32) Benzene-d6	5.031	84	332876	6.047	ug/L	-0.01
Spiked Amount	5.000	Range 70 - 125	Recovery	=	121.000%	
36) 1,2-Dichloropropane-d6	6.056	67	99381	5.791	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	115.800%	
41) Toluene-d8	7.294	98	237732	4.771	ug/L	-0.02
Spiked Amount	5.000	Range 70 - 130	Recovery	=	95.400%	
43) trans-1,3-Dichloroprop...	7.609	79	29245	4.718	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	94.400%	
46) 2-Hexanone-d5	8.101	63	116565	45.055	ug/L	0.02
Spiked Amount	50.000	Range 45 - 130	Recovery	=	90.100%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	55918	4.767	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	95.400%	
66) 1,2-Dichlorobenzene-d4	11.619	152	82035	5.365	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	107.200%	
Target Compounds					Qvalue	
13) Acetone	2.243	43	13920m	4.540	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092222\
Data File : VV028083.D
Acq On : 23 Sep 2022 01:09
Operator : SY/MD
Sample : N4621-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
CB8H3

Manual Integrations
APPROVED

Reviewed By :Krupa Patel 09/23/2022
Supervised By :Mahesh Dadoda 09/26/2022


Quant Time: Sep 23 04:54:01 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 23 04:38:54 2022
Response via : Initial Calibration

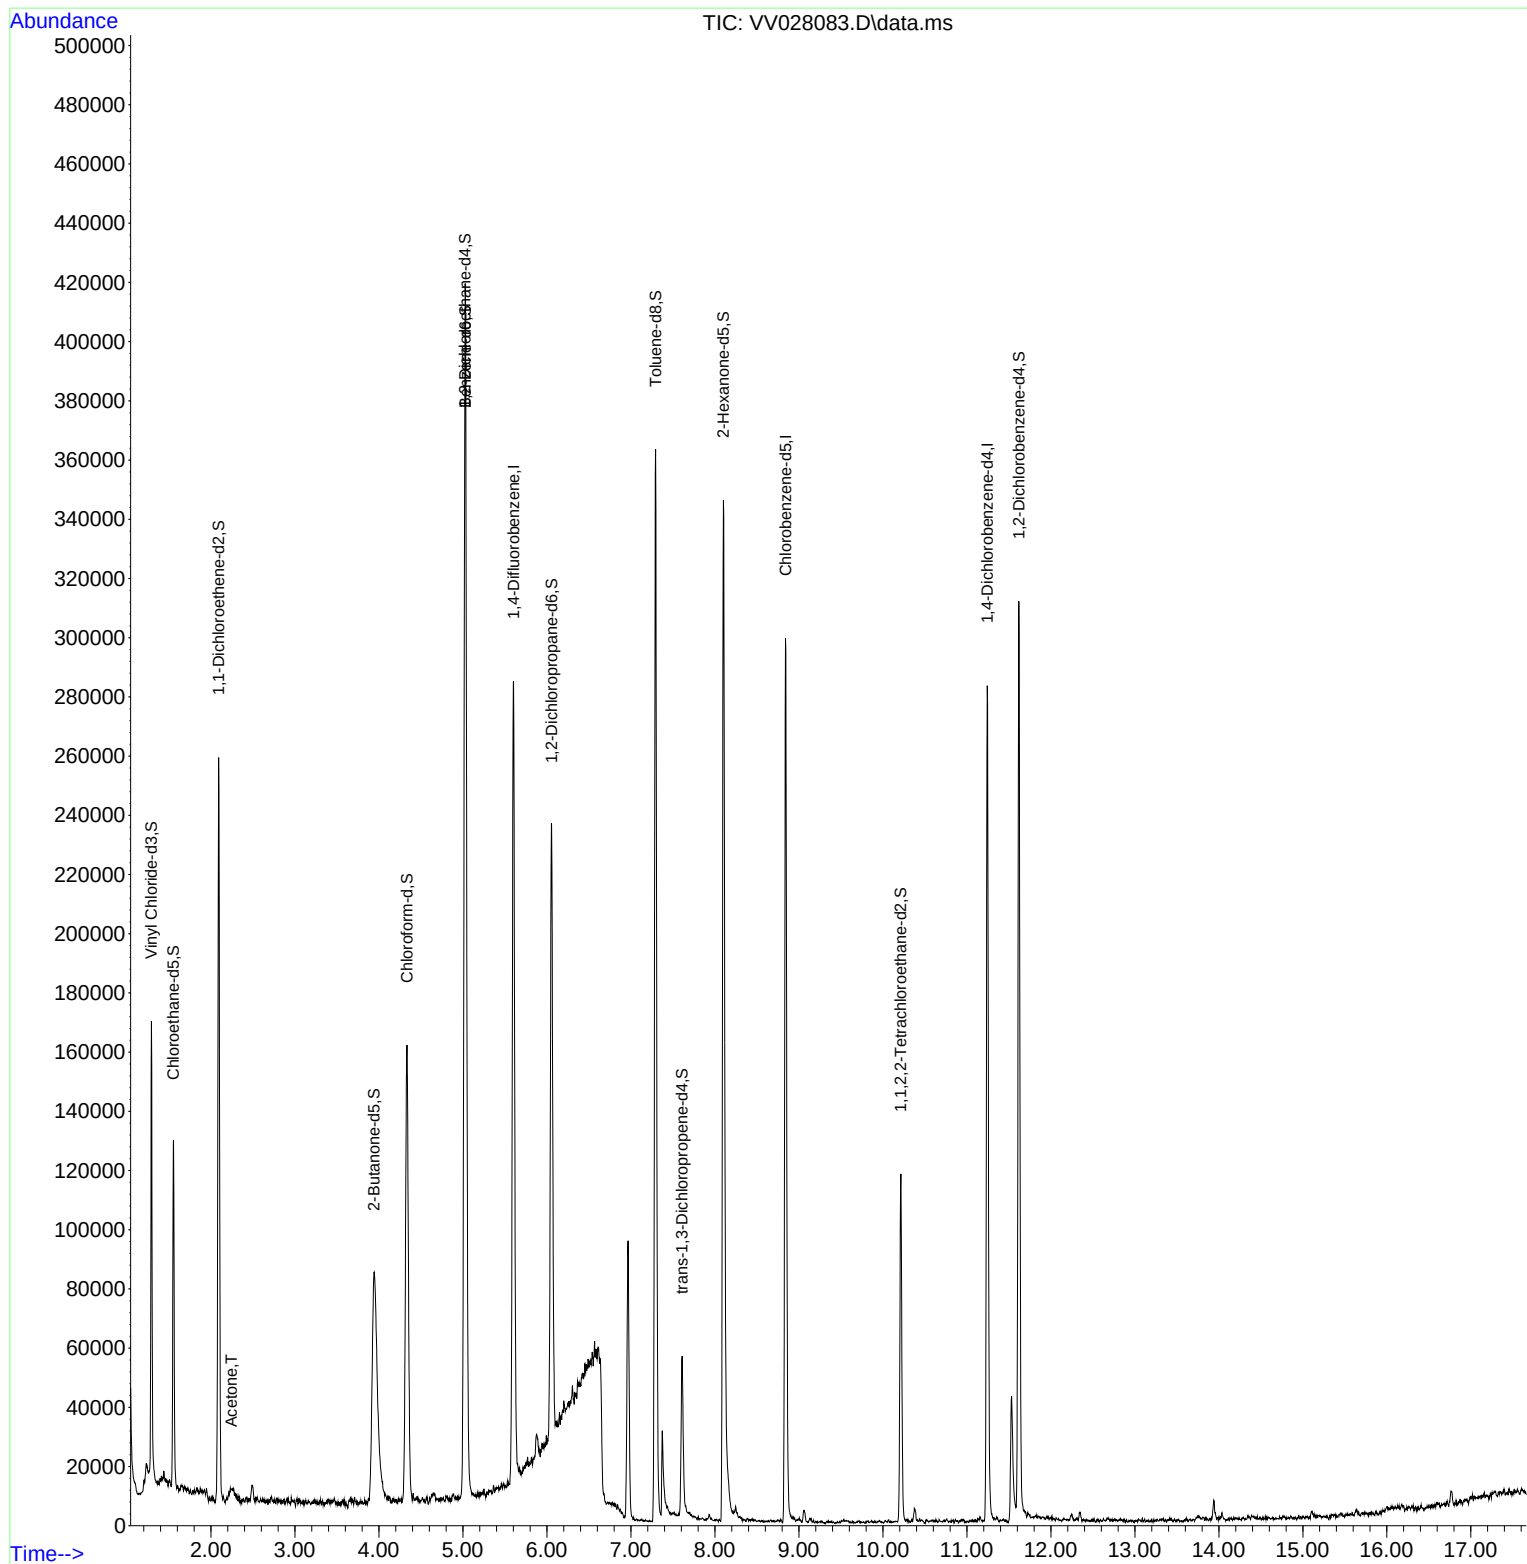

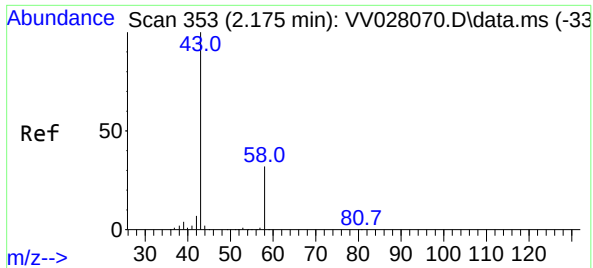

#13
Acetone
Concen: 4.540 ug/L m
RT: 2.243 min Scan# 31
Delta R.T. 0.068 min
Lab File: VV028083.D
Acq: 23 Sep 2022 01:09

Instrument :
MSVOA_V
ClientSampleId :
CB8H3

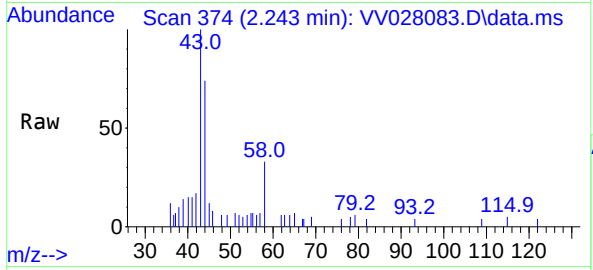

Tgt Ion: 43 Resp: 13920
Ion Ratio Lower Upper
43 100
58 0.8 0.0 65.6

Manual Integrations
APPROVED

Reviewed By :Krupa Patel 09/23/2022
Supervised By :Mahesh Dadoda 09/26/2022

