

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092222\
 Data File : VV028071.D
 Acq On : 22 Sep 2022 20:16
 Operator : SY/MD
 Sample : VV0922WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK233

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV028071.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	73	81	101	rVB	165506	182917	22.11%	2.773%
2	1.561	155	162	175	rBV	124893	142142	17.18%	2.155%
3	2.101	319	330	350	rVB	266448	386516	46.73%	5.859%
4	2.503	446	455	468	rVB3	6125	10476	1.27%	0.159%
5	3.889	875	886	919	rBV	81254	279652	33.81%	4.239%
6	4.342	1010	1027	1052	rBV	147074	369038	44.62%	5.594%
7	5.040	1228	1244	1271	rBV2	333804	827157	100.00%	12.539%
8	5.612	1410	1422	1452	rBV	201843	420367	50.82%	6.372%
9	6.066	1550	1563	1591	rBV	186112	389962	47.14%	5.911%
10	6.982	1836	1848	1868	rBV	92015	177875	21.50%	2.696%
11	7.313	1939	1951	1974	rBV	386085	694039	83.91%	10.521%
12	7.622	2036	2047	2064	rBV	54489	103429	12.50%	1.568%
13	8.088	2181	2192	2229	rBV	398086	787261	95.18%	11.934%
14	8.850	2416	2429	2455	rBV	327286	543561	65.71%	8.240%
15	10.214	2841	2853	2867	rBV	139329	220647	26.68%	3.345%
16	10.381	2895	2905	2914	rBV2	5655	9171	1.11%	0.139%
17	11.246	3163	3174	3191	rBV	311771	484052	58.52%	7.338%
18	11.535	3256	3264	3273	rBV7	7532	14395	1.74%	0.218%
19	11.622	3279	3291	3306	rBV	343618	554160	67.00%	8.400%




Sum of corrected areas: 6596817

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092222\
Data File : VV028071.D
Acq On : 22 Sep 2022 20:16
Operator : SY/MD
Sample : VV0922WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK233

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

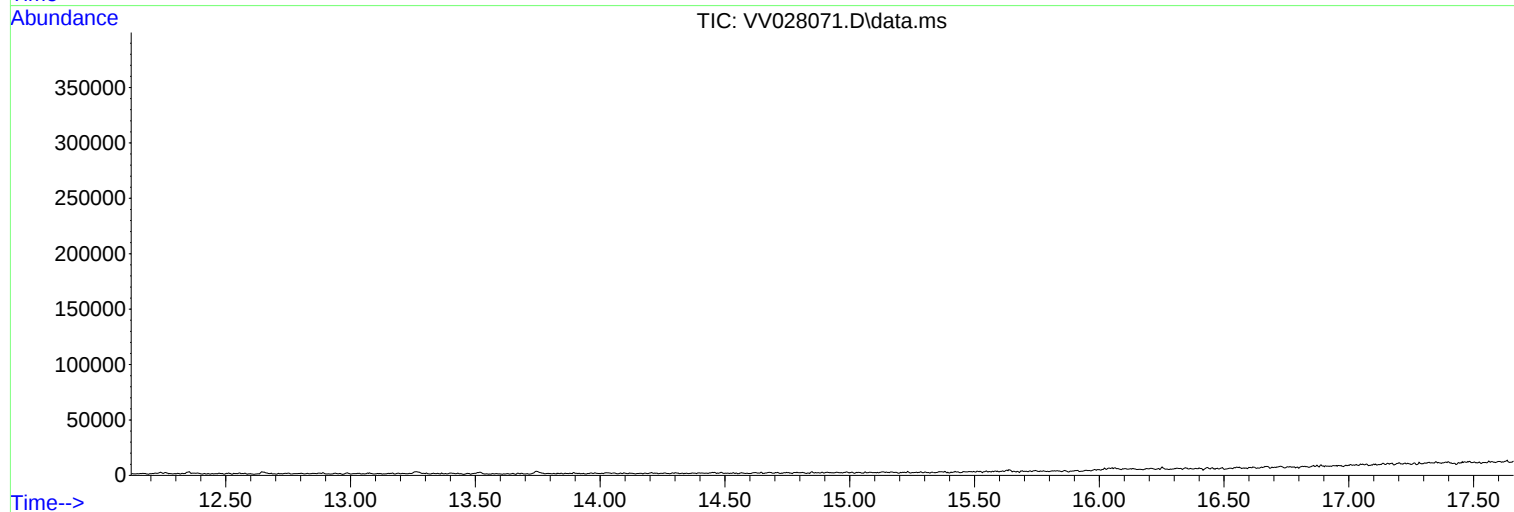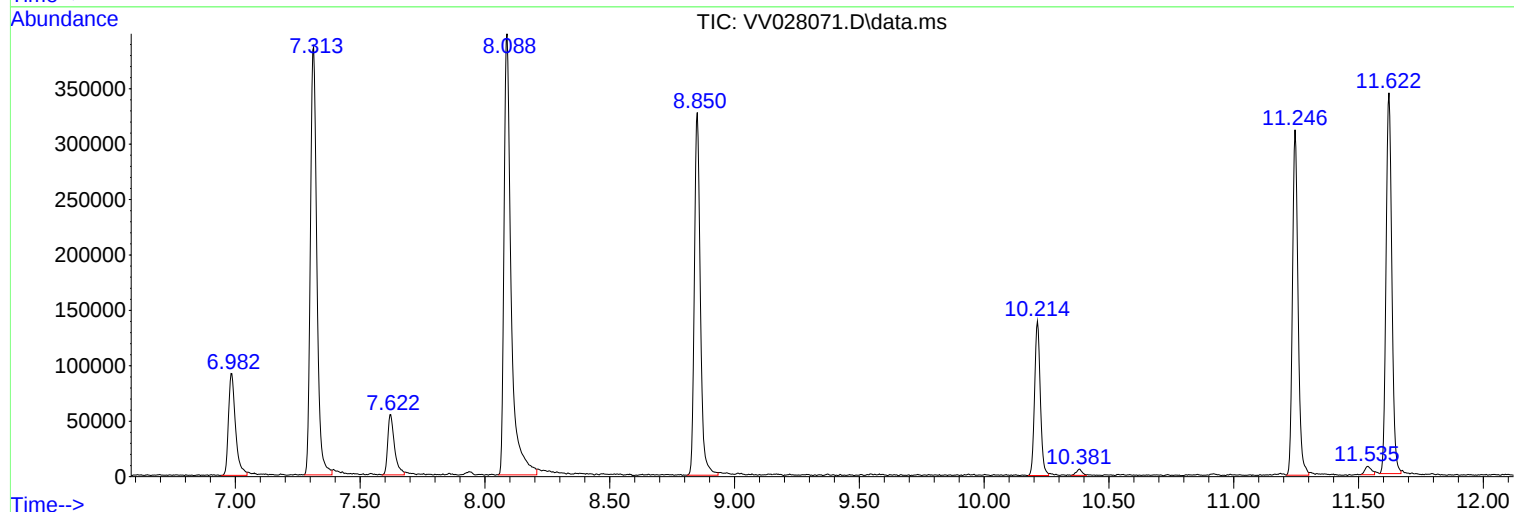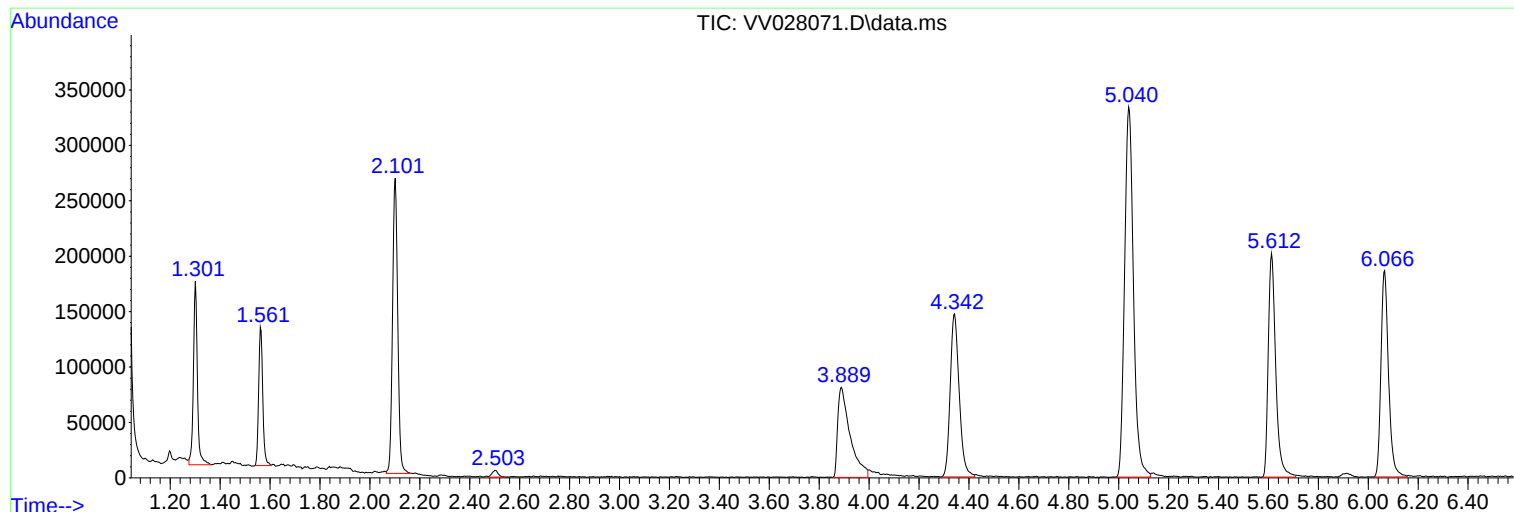

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092222\
Data File : VV028071.D
Acq On : 22 Sep 2022 20:16
Operator : SY/MD
Sample : VV0922WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK233

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092222\
Data File : VV028071.D
Acq On : 22 Sep 2022 20:16
Operator : SY/MD
Sample : VV0922WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK233

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc