

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092222\
 Data File : VV028072.D
 Acq On : 22 Sep 2022 20:40
 Operator : SY/MD
 Sample : N4652-09DL 40X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ32DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV028072.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	74	81	96	rVB2	200489	221608	28.23%	3.128%
2	1.561	155	162	176	rBV2	121363	172823	22.01%	2.440%
3	2.101	318	330	348	rVB	255687	372673	47.47%	5.261%
4	2.503	444	455	468	rVB	20218	33118	4.22%	0.468%
5	3.182	649	666	693	rBV	142609	307628	39.19%	4.343%
6	3.902	872	890	925	rBV3	188214	627758	79.96%	8.862%
7	4.342	1009	1027	1053	rBV	137600	342748	43.66%	4.839%
8	4.600	1094	1107	1124	rBV4	15440	38755	4.94%	0.547%
9	5.040	1228	1244	1271	rBV3	317982	785055	100.00%	11.083%
10	5.612	1409	1422	1445	rBV	202328	418398	53.30%	5.907%
11	5.918	1504	1517	1529	rVB	4615	11793	1.50%	0.166%
12	6.066	1549	1563	1586	rBV	176075	368833	46.98%	5.207%
13	6.985	1837	1849	1873	rBV	80000	155916	19.86%	2.201%
14	7.313	1939	1951	1972	rBV	359441	651332	82.97%	9.195%
15	7.622	2038	2047	2069	rBV	52207	98234	12.51%	1.387%
16	8.088	2180	2192	2234	rBV	362660	724770	92.32%	10.232%
17	8.850	2417	2429	2445	rBV	324107	537333	68.45%	7.586%
18	10.214	2840	2853	2867	rBV	129279	205195	26.14%	2.897%
19	11.246	3163	3174	3190	rBV	305778	481459	61.33%	6.797%
20	11.622	3279	3291	3311	rBV	330463	528211	67.28%	7.457%




Sum of corrected areas: 7083640

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092222\
Data File : VV028072.D
Acq On : 22 Sep 2022 20:40
Operator : SY/MD
Sample : N4652-09DL 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ32DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

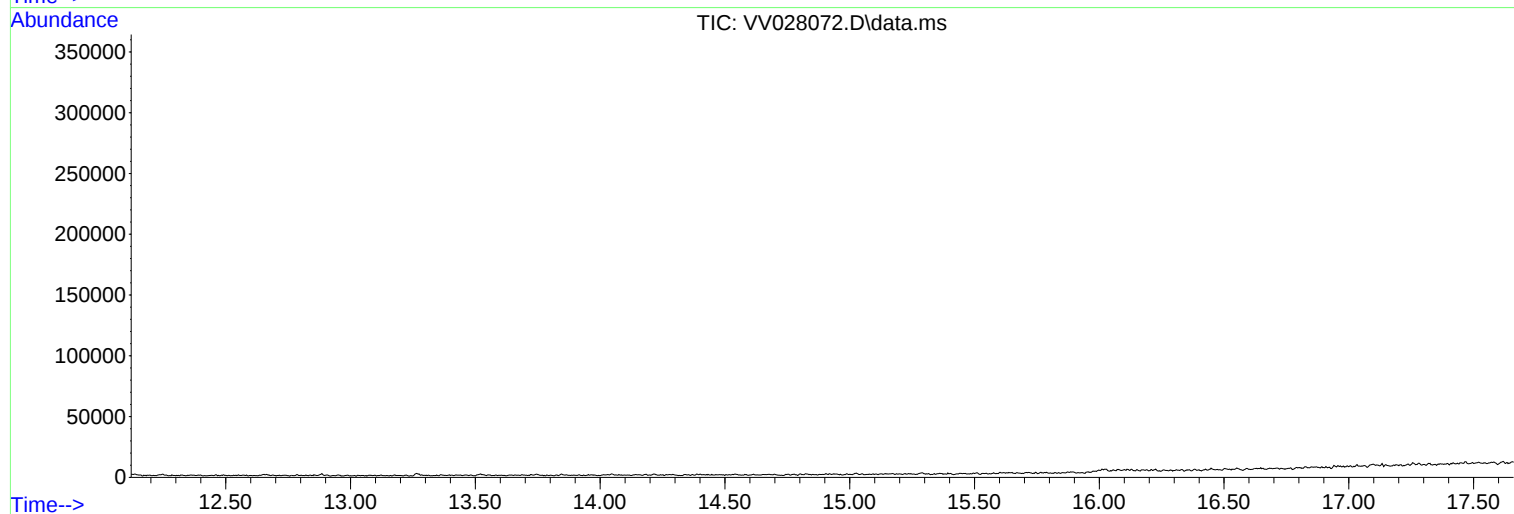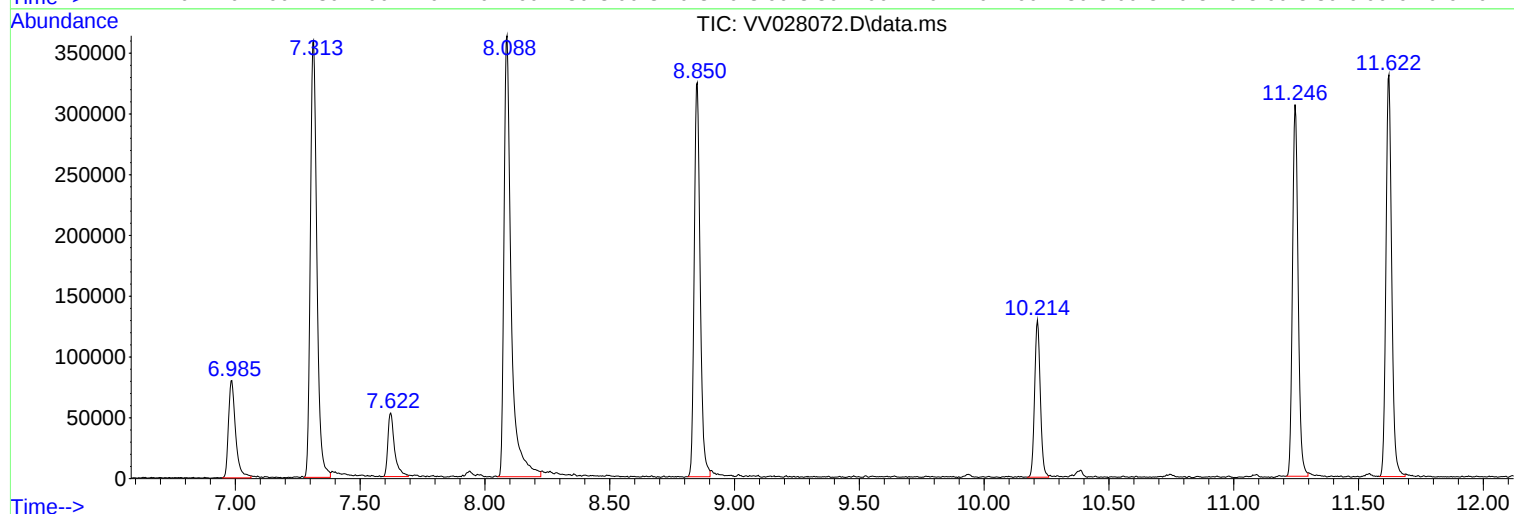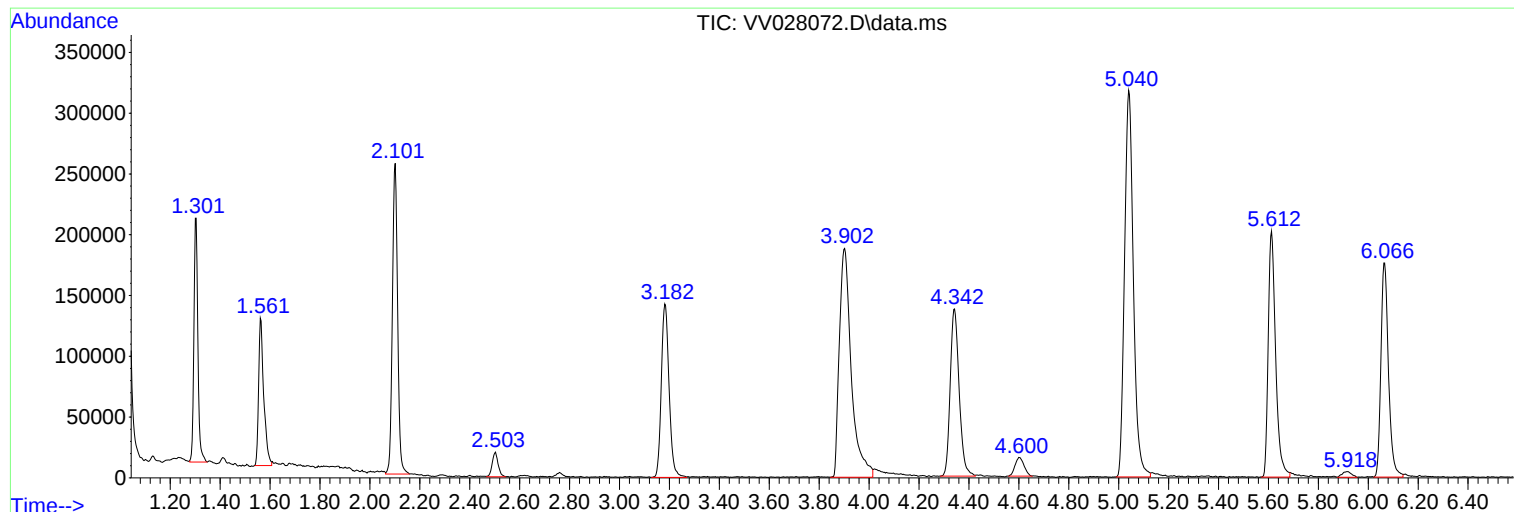

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092222\
Data File : VV028072.D
Acq On : 22 Sep 2022 20:40
Operator : SY/MD
Sample : N4652-09DL 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ32DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092222\
Data File : VV028072.D
Acq On : 22 Sep 2022 20:40
Operator : SY/MD
Sample : N4652-09DL 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ32DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
