

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092222\
 Data File : VV028073.D
 Acq On : 22 Sep 2022 21:05
 Operator : SY/MD
 Sample : N4652-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ29

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV028073.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	98	rVB	153383	158315	20.34%	2.576%
2	1.561	155	162	173	rBV	119215	134349	17.26%	2.186%
3	2.101	320	330	344	rBV	247720	359124	46.13%	5.843%
4	3.876	873	882	915	rBV	91340	264570	33.99%	4.304%
5	4.342	1011	1027	1056	rBV	137273	350309	45.00%	5.699%
6	4.603	1094	1108	1125	rVB4	14538	34978	4.49%	0.569%
7	5.040	1227	1244	1275	rBV2	307960	778485	100.00%	12.666%
8	5.613	1410	1422	1444	rBV	195939	402230	51.67%	6.544%
9	6.066	1549	1563	1581	rBV2	172846	357623	45.94%	5.818%
10	6.982	1837	1848	1868	rBV2	81279	153829	19.76%	2.503%
11	7.313	1937	1951	1973	rBV	351163	623864	80.14%	10.150%
12	7.622	2037	2047	2068	rBV	49948	91107	11.70%	1.482%
13	7.973	2147	2156	2174	rVB3	34007	60249	7.74%	0.980%
14	8.085	2179	2191	2225	rBV	340376	662921	85.16%	10.786%
15	8.850	2413	2429	2453	rBV	307362	512505	65.83%	8.338%
16	10.214	2841	2853	2866	rBV	124817	195155	25.07%	3.175%
17	10.381	2895	2905	2921	rVB3	7258	14574	1.87%	0.237%
18	11.246	3157	3174	3198	rBV	303012	475960	61.14%	7.744%
19	11.622	3279	3291	3311	rBV	321100	516257	66.32%	8.399%




Sum of corrected areas: 6146404

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092222\
Data File : VV028073.D
Acq On : 22 Sep 2022 21:05
Operator : SY/MD
Sample : N4652-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ29

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

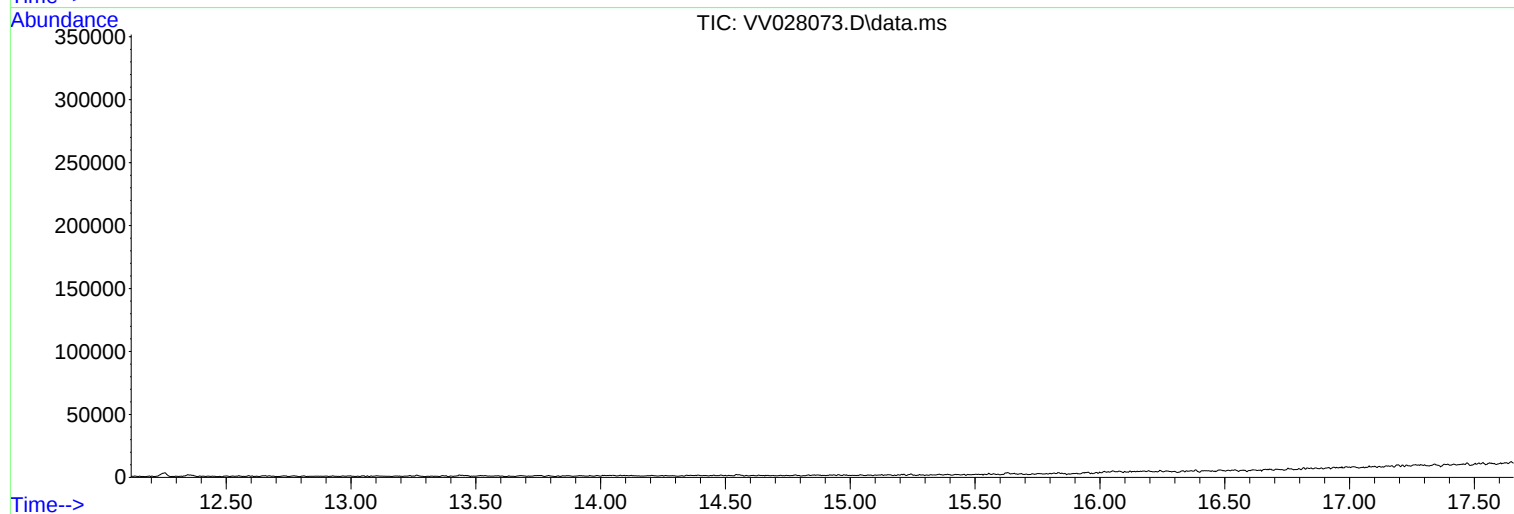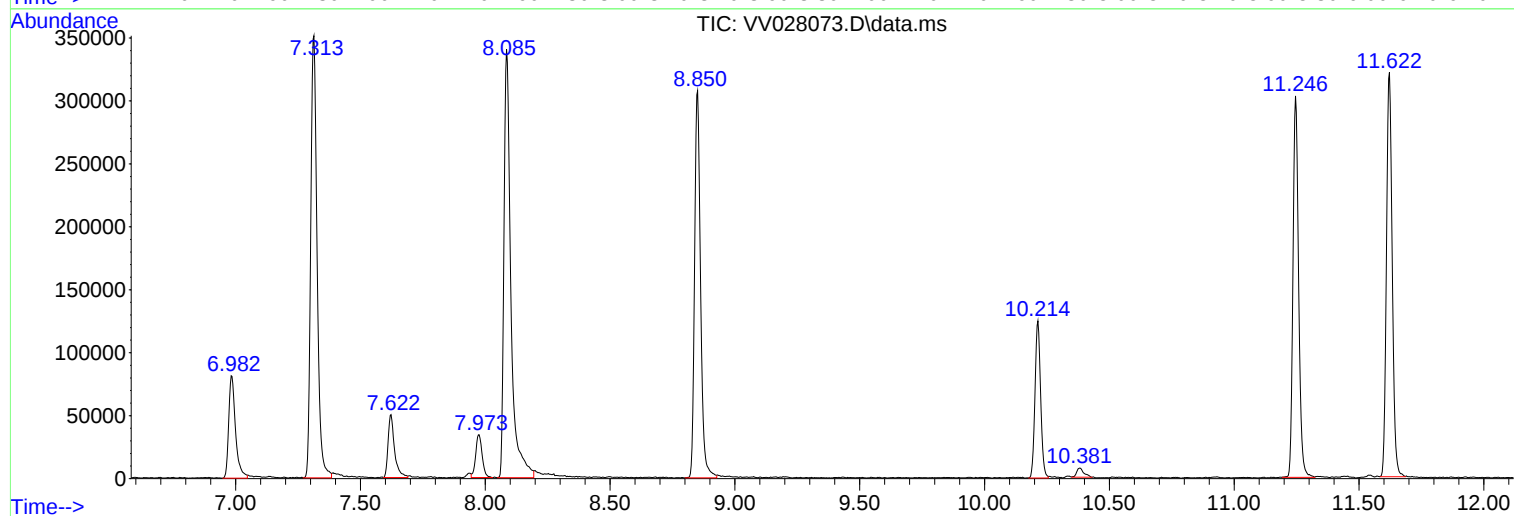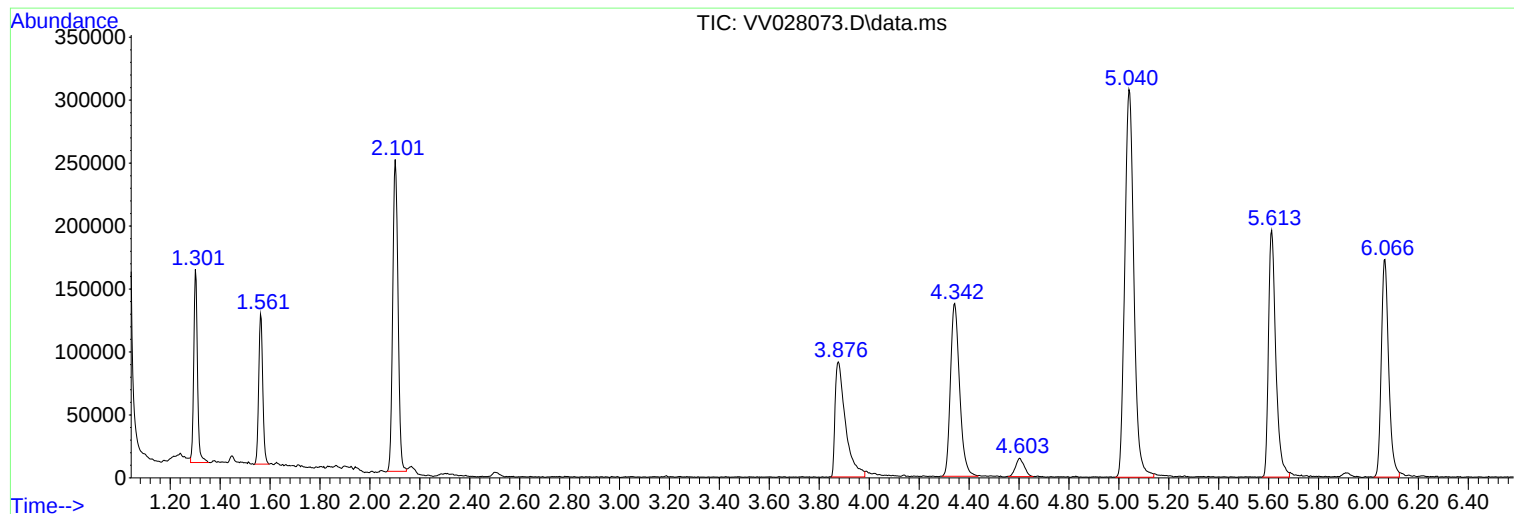

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092222\
Data File : VV028073.D
Acq On : 22 Sep 2022 21:05
Operator : SY/MD
Sample : N4652-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ29

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092222\
Data File : VV028073.D
Acq On : 22 Sep 2022 21:05
Operator : SY/MD
Sample : N4652-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ29

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------