

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092222\
 Data File : VV028076.D
 Acq On : 22 Sep 2022 22:18
 Operator : SY/MD
 Sample : N4652-05DL 20X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ18DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV028076.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	96	rVB	150466	153641	18.58%	2.282%
2	1.561	155	162	173	rBV	115905	134826	16.30%	2.003%
3	2.101	318	330	345	rBV	250935	357633	43.25%	5.312%
4	2.288	376	388	405	rBV	183368	273187	33.04%	4.058%
5	2.500	442	454	467	rBV2	22228	38468	4.65%	0.571%
6	3.892	868	887	922	rBV2	92027	378046	45.72%	5.616%
7	4.342	1010	1027	1050	rBV	147273	368930	44.62%	5.480%
8	5.040	1229	1244	1270	rBV2	329496	826911	100.00%	12.283%
9	5.613	1405	1422	1448	rBV	204547	422844	51.14%	6.281%
10	6.066	1550	1563	1582	rBV	179959	373782	45.20%	5.552%
11	6.982	1838	1848	1868	rBV	84587	162453	19.65%	2.413%
12	7.313	1936	1951	1973	rBV	363120	650029	78.61%	9.656%
13	7.622	2037	2047	2067	rBV	52018	97151	11.75%	1.443%
14	7.934	2131	2144	2154	rBV2	8933	16068	1.94%	0.239%
15	8.088	2181	2192	2235	rBV	367187	731328	88.44%	10.864%
16	8.850	2413	2429	2452	rBV	314105	529301	64.01%	7.863%
17	10.214	2841	2853	2870	rBV2	131458	210333	25.44%	3.124%
18	10.378	2896	2904	2916	rBV2	16673	27656	3.34%	0.411%
19	11.246	3162	3174	3191	rBV	293734	460415	55.68%	6.839%
20	11.622	3279	3291	3310	rBV	317919	508400	61.48%	7.552%
21	12.246	3476	3485	3496	rVB2	5783	10553	1.28%	0.157%


Sum of corrected areas: 6731955

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092222\
Data File : VV028076.D
Acq On : 22 Sep 2022 22:18
Operator : SY/MD
Sample : N4652-05DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ18DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

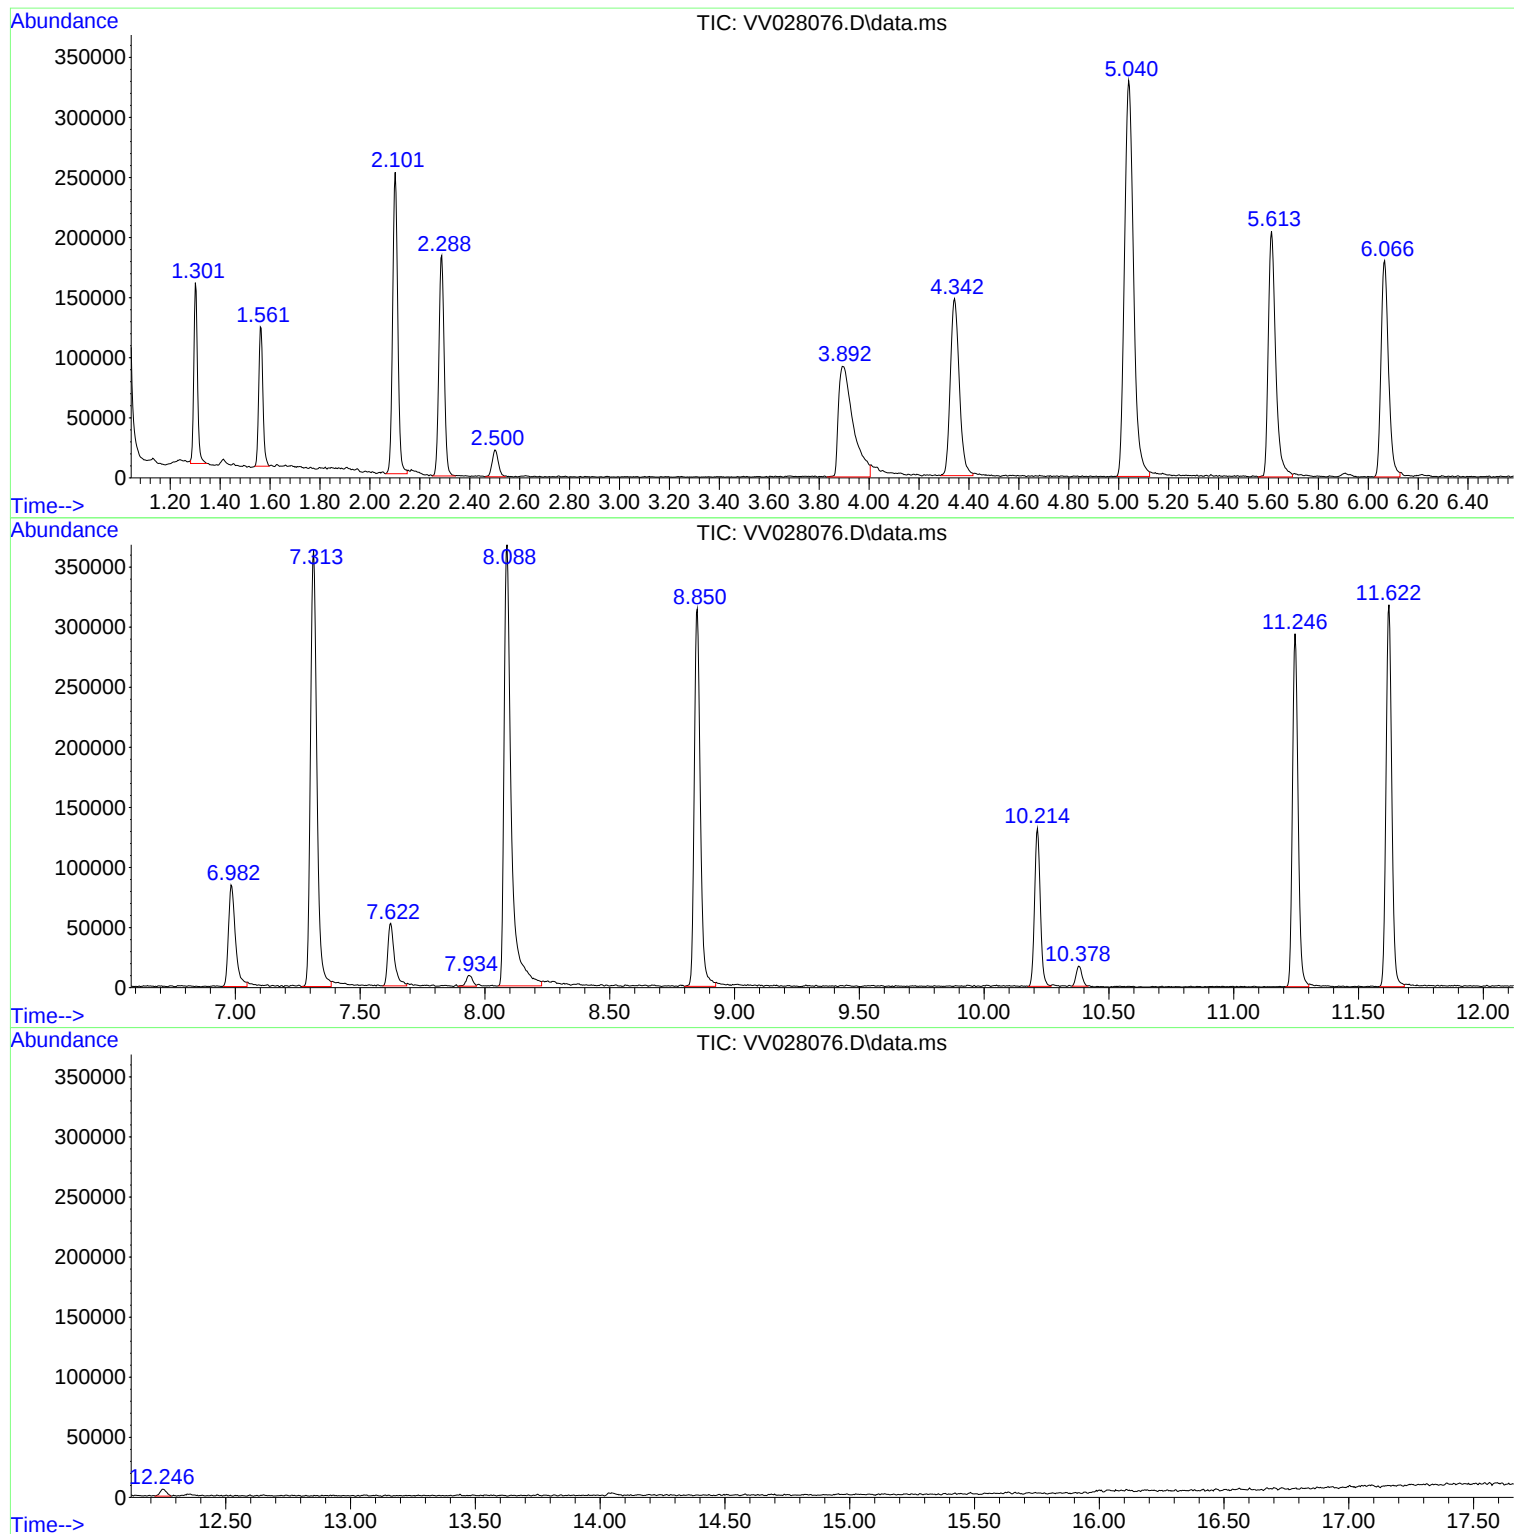

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092222\
Data File : VV028076.D
Acq On : 22 Sep 2022 22:18
Operator : SY/MD
Sample : N4652-05DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ18DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092222\
Data File : VV028076.D
Acq On : 22 Sep 2022 22:18
Operator : SY/MD
Sample : N4652-05DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ18DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc