

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092222\
 Data File : VV028078.D
 Acq On : 22 Sep 2022 23:07
 Operator : SY/MD
 Sample : N4652-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV028078.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	95	rVB	144300	150803	19.29%	2.334%
2	1.561	155	162	174	rVB	117565	135209	17.30%	2.093%
3	2.101	318	330	342	rBV	234929	335520	42.92%	5.193%
4	2.503	444	455	465	rBV2	22352	36173	4.63%	0.560%
5	3.873	868	881	912	rBV2	103616	314808	40.27%	4.873%
6	4.343	1010	1027	1048	rBV	143216	356541	45.61%	5.519%
7	5.043	1227	1245	1276	rBV2	307012	781711	100.00%	12.100%
8	5.613	1411	1422	1450	rBV	230427	472416	60.43%	7.312%
9	6.066	1547	1563	1588	rBV	186894	395956	50.65%	6.129%
10	6.986	1837	1849	1866	rBV	82737	157612	20.16%	2.440%
11	7.314	1940	1951	1974	rBV	358939	633894	81.09%	9.812%
12	7.619	2035	2046	2067	rBV	47919	88741	11.35%	1.374%
13	7.937	2133	2145	2155	rBV3	7446	14585	1.87%	0.226%
14	8.085	2180	2191	2225	rBV	335183	649240	83.05%	10.049%
15	8.420	2285	2295	2304	rBV6	4439	8486	1.09%	0.131%
16	8.850	2418	2429	2455	rBV	369792	620881	79.43%	9.610%
17	10.214	2839	2853	2868	rBV	127368	205595	26.30%	3.182%
18	10.381	2896	2905	2916	rVB3	11175	18460	2.36%	0.286%
19	11.246	3163	3174	3198	rBV	357110	558769	71.48%	8.649%
20	11.622	3279	3291	3313	rBV	328167	525115	67.18%	8.128%




Sum of corrected areas: 6460515

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092222\
Data File : VV028078.D
Acq On : 22 Sep 2022 23:07
Operator : SY/MD
Sample : N4652-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

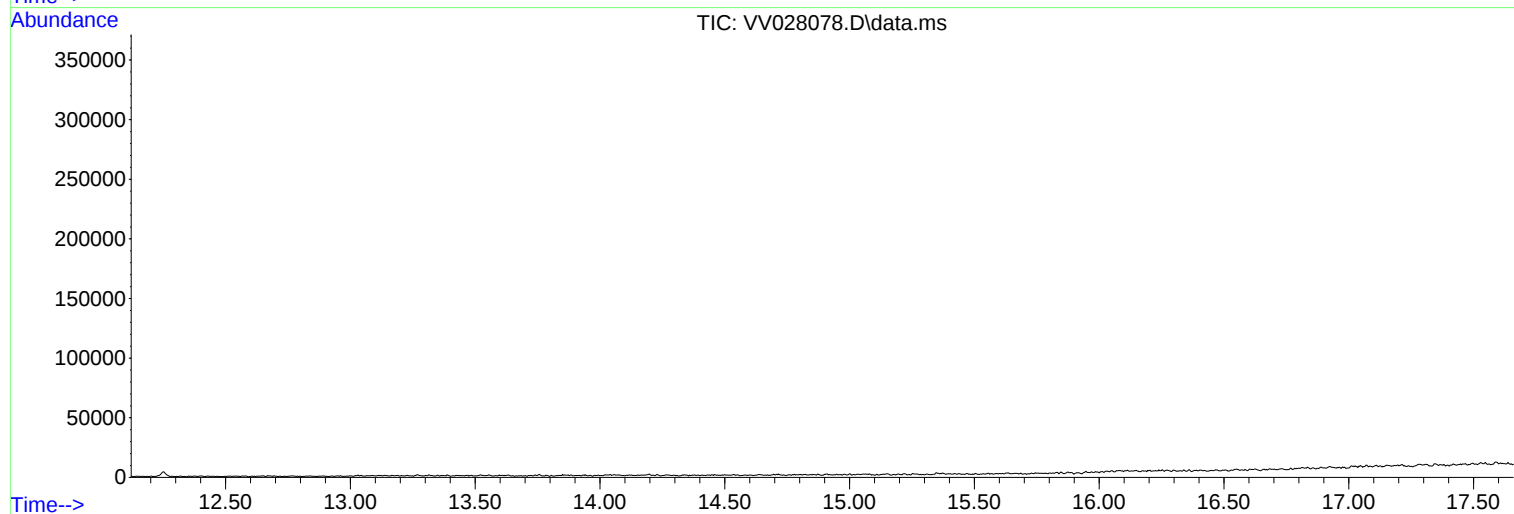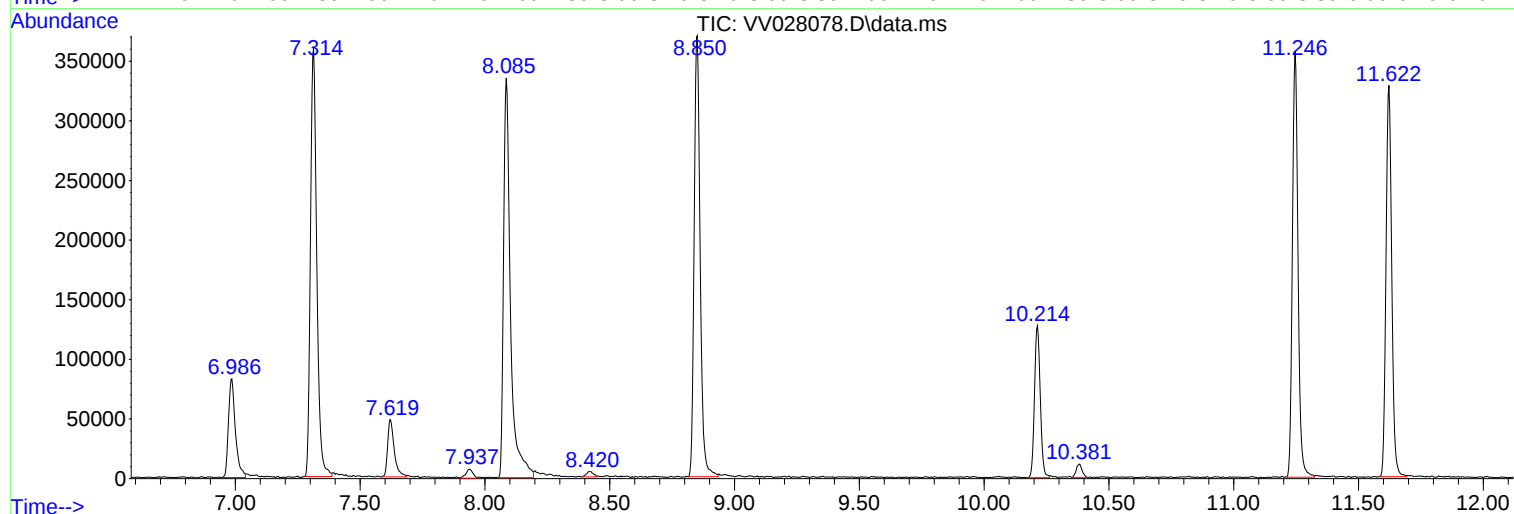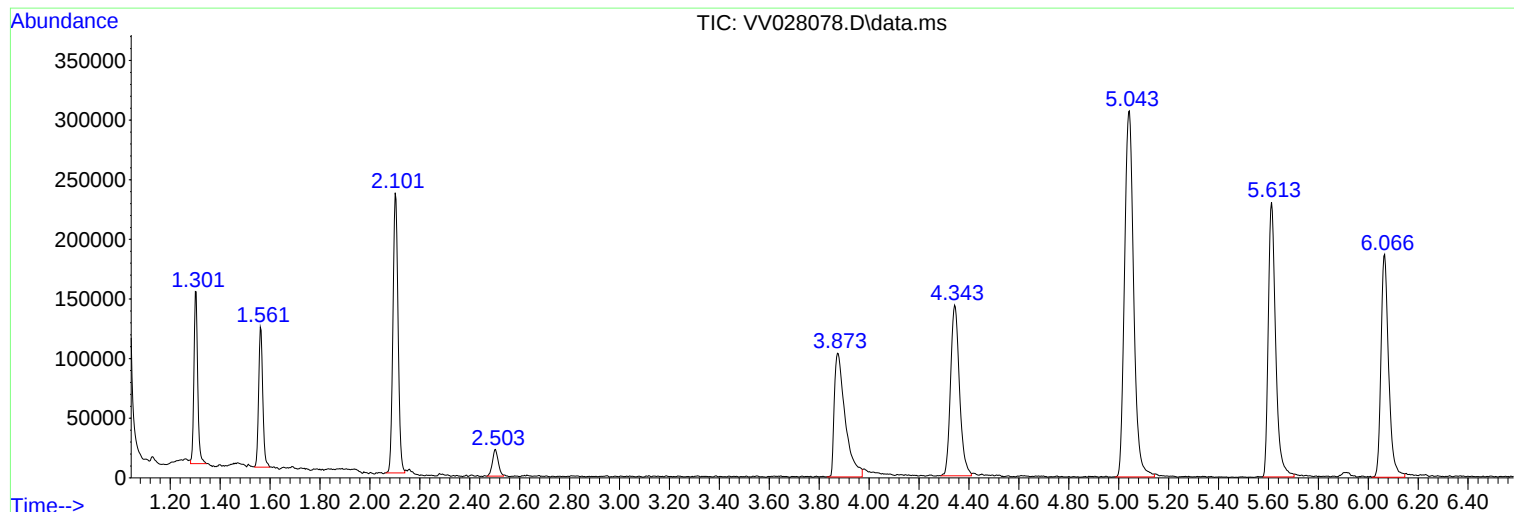

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092222\
Data File : VV028078.D
Acq On : 22 Sep 2022 23:07
Operator : SY/MD
Sample : N4652-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092222\
Data File : VV028078.D
Acq On : 22 Sep 2022 23:07
Operator : SY/MD
Sample : N4652-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc