

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092222\
 Data File : VV028079.D
 Acq On : 22 Sep 2022 23:31
 Operator : SY/MD
 Sample : N4621-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB8G4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV028079.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.237	56	61	74	rVB2	11575	17179	2.26%	0.279%
2	1.301	75	81	92	rVB	142564	142641	18.76%	2.314%
3	1.561	155	162	181	rVB	118021	138510	18.22%	2.247%
4	2.011	296	302	309	rVB4	7039	9633	1.27%	0.156%
5	2.101	318	330	342	rBV	241662	347448	45.70%	5.638%
6	2.163	342	349	364	rVB2	9293	20001	2.63%	0.325%
7	2.291	377	389	411	rBV	42596	108856	14.32%	1.766%
8	3.873	871	881	916	rBV	86360	251281	33.05%	4.077%
9	4.343	1010	1027	1062	rBV2	134571	340947	44.84%	5.532%
10	5.040	1228	1244	1273	rBV3	303351	760294	100.00%	12.336%
11	5.613	1411	1422	1452	rVV	202078	412610	54.27%	6.695%
12	5.905	1504	1513	1525	rBV9	5068	9484	1.25%	0.154%
13	6.066	1547	1563	1584	rBV	171531	358028	47.09%	5.809%
14	6.982	1838	1848	1868	rBV2	78312	146693	19.29%	2.380%
15	7.314	1938	1951	1973	rBV	339542	604369	79.49%	9.806%
16	7.622	2034	2047	2070	rBV	48395	90332	11.88%	1.466%
17	7.934	2136	2144	2158	rVB3	5086	9311	1.22%	0.151%
18	8.085	2179	2191	2226	rBV	326095	631606	83.07%	10.248%
19	8.432	2290	2299	2310	rBV5	11361	20243	2.66%	0.328%
20	8.850	2416	2429	2451	rBV	313888	523663	68.88%	8.497%
21	10.214	2841	2853	2871	rBV	117590	186861	24.58%	3.032%
22	10.381	2896	2905	2918	rVB2	16766	29382	3.86%	0.477%
23	11.246	3163	3174	3196	rBV	307352	482846	63.51%	7.834%
24	11.622	3277	3291	3309	rBV	317566	501896	66.01%	8.144%
25	12.252	3477	3487	3498	rVB3	4739	7842	1.03%	0.127%
26	12.349	3505	3517	3526	rBV9	6462	11181	1.47%	0.181%




Sum of corrected areas: 6163137

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092222\
Data File : VV028079.D
Acq On : 22 Sep 2022 23:31
Operator : SY/MD
Sample : N4621-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB8G4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

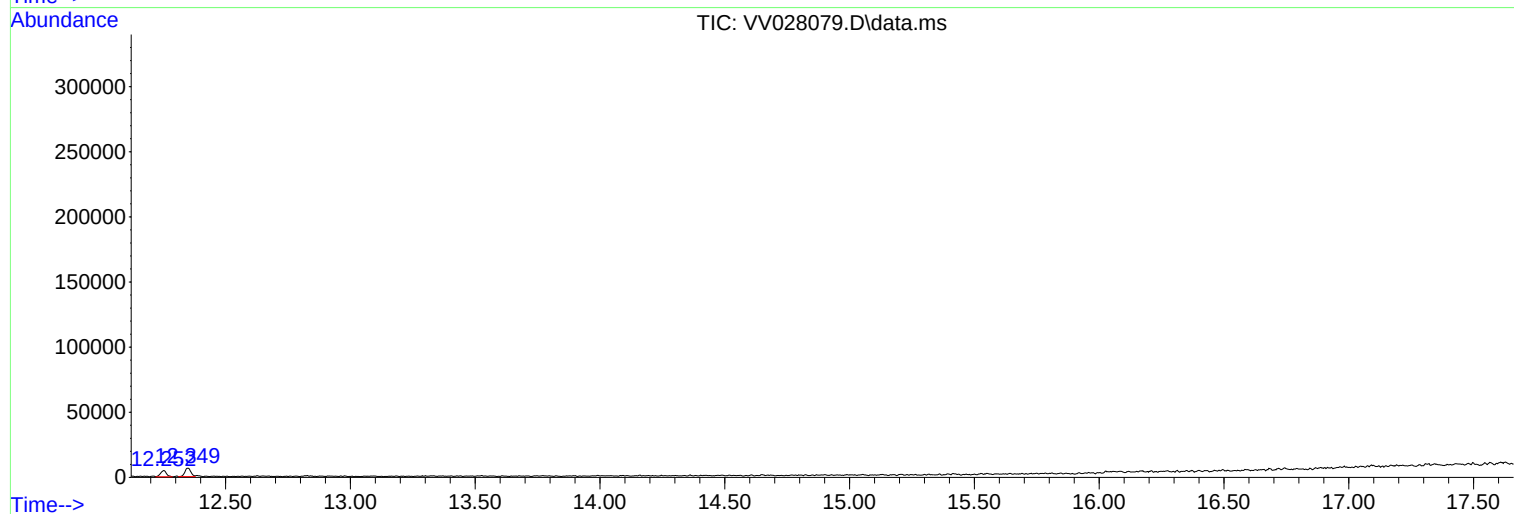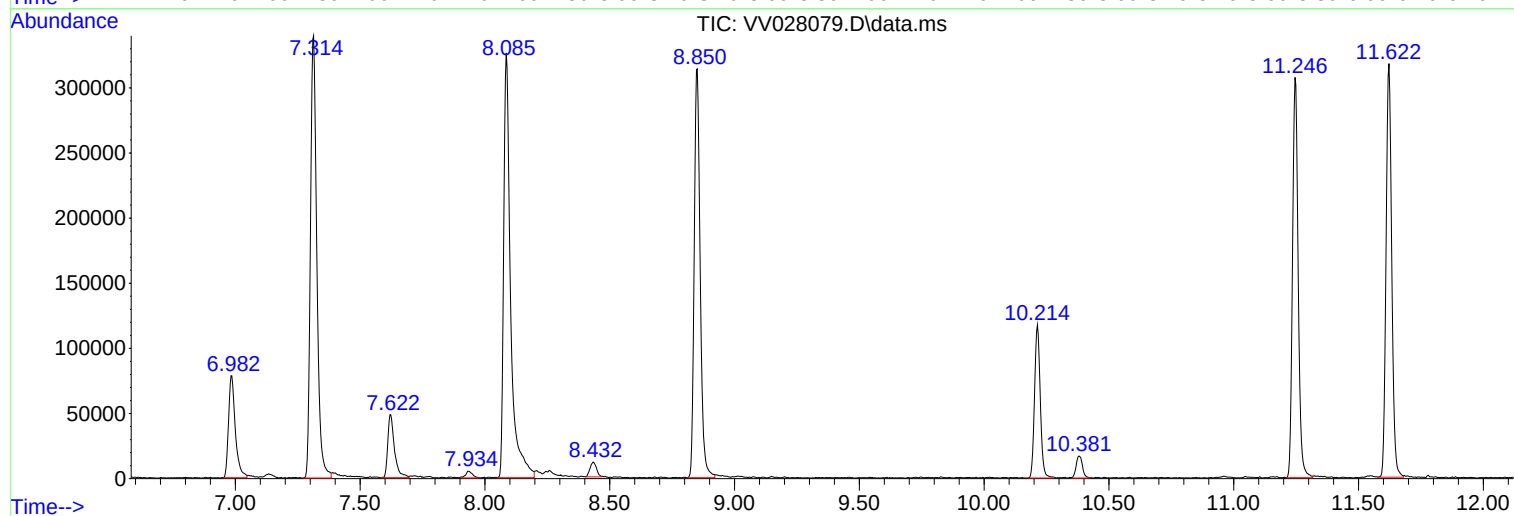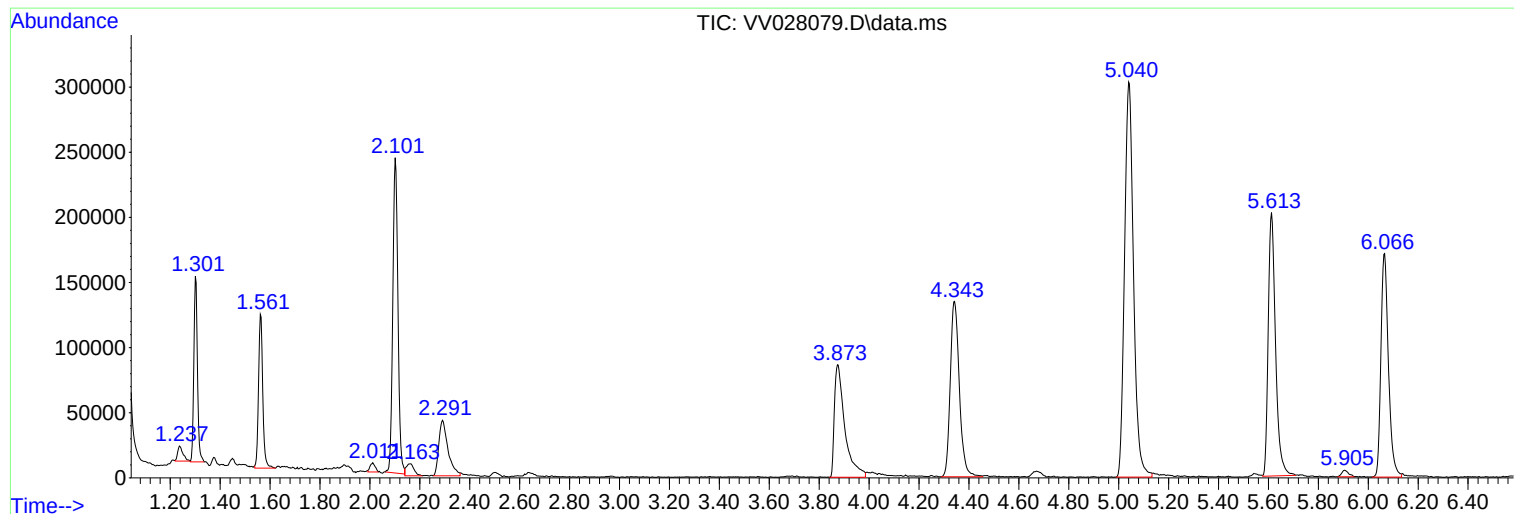

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092222\
Data File : VV028079.D
Acq On : 22 Sep 2022 23:31
Operator : SY/MD
Sample : N4621-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB8G4










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.291	1.32 ug/L	108856	1,4-Difluorobenzene	5.613

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	78
2			Isopropyl Alcohol	60	C3H8O	000067-63-0	78
3			Isopropyl Alcohol	60	C3H8O	000067-63-0	56
4			Isopropyl Alcohol	60	C3H8O	000067-63-0	56
5			Propane, 2-ethoxy-	88	C5H12O	000625-54-7	56

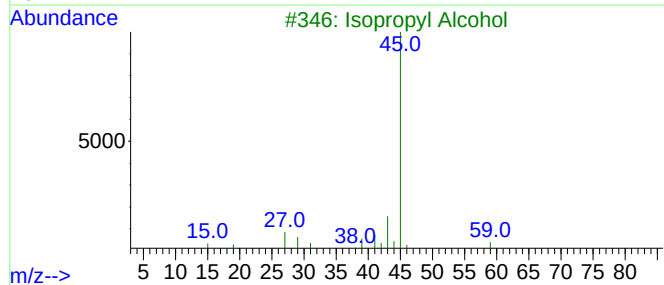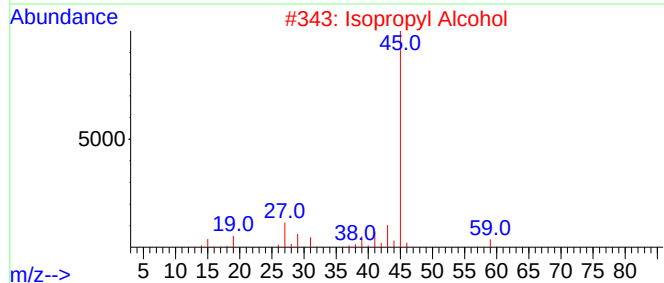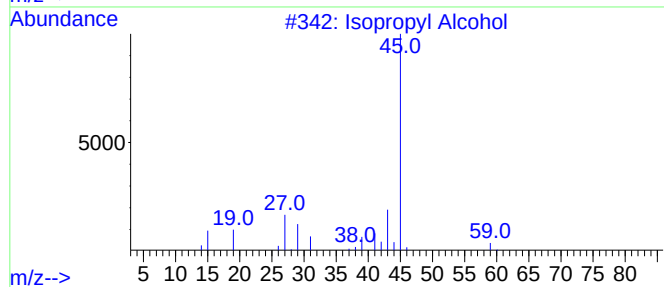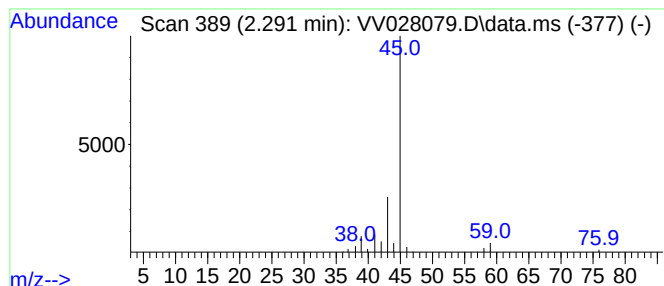

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092222\
Data File : VV028079.D
Acq On : 22 Sep 2022 23:31
Operator : SY/MD
Sample : N4621-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB8G4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.291	1.3	ug/L	108856	1	5.613	412610	5.0