


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092222\
Data File : VV028061.D
Acq On : 22 Sep 2022 13:58
Operator : SY/MD
Sample : BFB374
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB374

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Mon Sep 26 21:28:54 2022

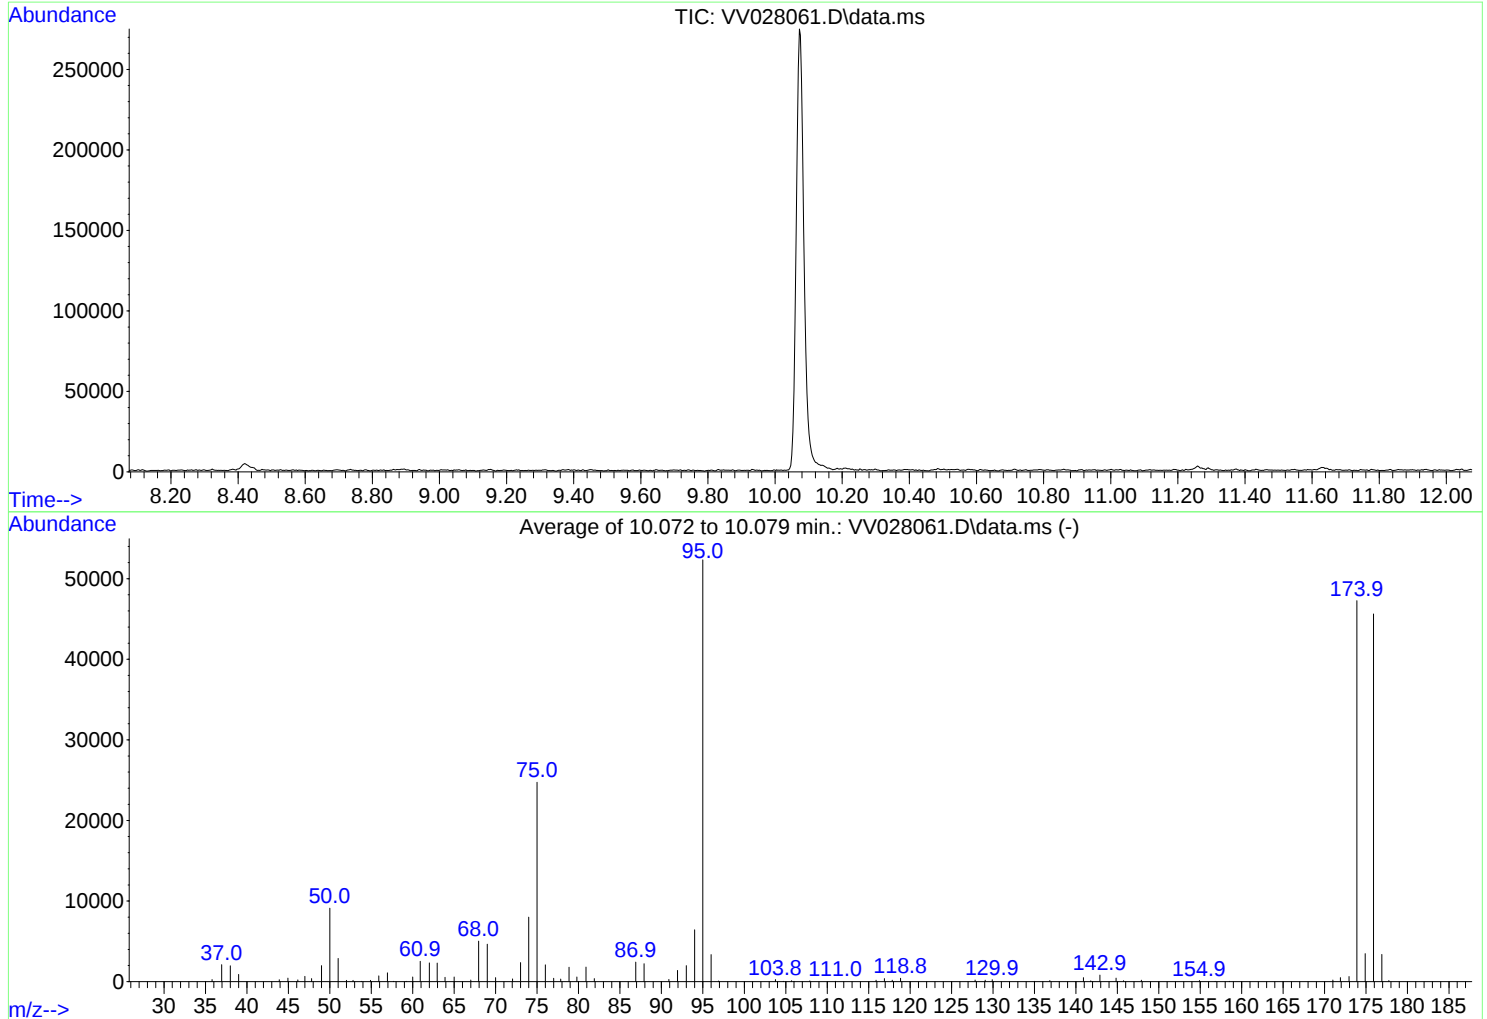

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	9117	PASS
75	95	30	80	47.3	24747	PASS
95	95	100	100	100.0	52339	PASS
96	95	5	9	6.4	3350	PASS
173	174	0.00	2	1.4	642	PASS
174	95	50	120	90.3	47269	PASS
175	174	5	9	7.3	3469	PASS
176	174	95	105	96.5	45621	PASS
177	176	5	10	7.4	3372	PASS

Scan 2797 (10.034 min): VV028061.D\data.ms
BFB374

m/z	Abundance
35.80	107.0
39.90	366.0
43.00	130.0
43.90	430.0

Instrument :
MSVOA_V
ClientSampleId :
BFB374

m/z	Abundance
35.90	389.0
37.00	2144.0
38.00	1967.0
39.00	991.0
39.90	339.0
44.00	675.0
44.90	427.0
46.10	190.0
47.00	809.0
47.80	395.0
49.00	2067.0
50.00	9608.0
51.00	3213.0
52.00	141.0
52.80	133.0
53.80	110.0
54.90	165.0
55.90	644.0
57.00	1144.0
60.00	594.0
60.90	2703.0
62.00	2539.0
63.00	2494.0
63.90	628.0
65.00	567.0
67.00	229.0
68.00	5269.0
69.00	5159.0
70.00	502.0
72.00	317.0
73.00	2511.0
74.00	8592.0
75.00	26720.0
76.00	2311.0
77.00	460.0
77.80	350.0
78.90	1811.0
79.80	630.0
80.90	1837.0
81.90	373.0
86.90	2496.0
87.90	2545.0
90.90	262.0
92.00	1400.0
93.00	2211.0
94.00	6795.0
95.00	54152.0
96.00	3525.0
96.90	145.0
103.80	279.0
105.70	194.0
107.90	152.0
111.00	136.0
115.90	209.0
116.90	421.0
117.90	236.0
118.80	391.0
127.90	192.0
129.00	158.0
129.90	240.0
136.90	179.0
140.90	543.0
142.90	824.0
144.90	418.0
145.70	137.0
147.90	190.0
154.90	121.0
156.80	109.0
171.10	188.0
171.90	514.0
173.00	659.0
173.90	48408.0
174.90	3656.0
175.90	47232.0
176.90	3520.0
177.80	126.0

Instrument :
MSVOA_V
ClientSampleId :
BFB374

m/z	Abundance
35.80	352.0
36.90	2152.0
38.00	2057.0
39.00	893.0
39.90	319.0
43.00	137.0
43.90	711.0
44.90	463.0
46.10	237.0
47.00	671.0
47.80	385.0
49.00	2028.0
50.00	9482.0
51.00	2981.0
52.00	159.0
52.80	164.0
54.90	162.0
55.90	735.0
56.90	1085.0
57.70	109.0
59.20	104.0
60.00	603.0
60.90	2590.0
62.00	2392.0
63.00	2328.0
63.90	557.0
65.00	597.0
67.00	227.0
67.90	5196.0
69.00	4712.0
70.00	522.0
72.00	346.0
73.00	2455.0
74.00	8211.0
75.00	25504.0
76.00	2114.0
77.00	445.0
77.90	349.0
78.90	1885.0
79.80	592.0
80.90	1864.0
81.90	385.0
86.90	2539.0
87.90	2254.0
90.90	276.0
91.90	1377.0
93.00	2011.0
94.00	6628.0
95.00	54312.0
96.00	3408.0
96.90	101.0
103.70	282.0
105.70	169.0
107.90	131.0
115.80	167.0
116.90	399.0
117.80	182.0
118.80	435.0
127.90	191.0
129.00	197.0
129.90	236.0
136.90	148.0
140.90	517.0
141.80	115.0
142.90	843.0
144.80	457.0
145.70	117.0
147.90	197.0
154.90	151.0
171.00	199.0
171.90	532.0
172.90	645.0
173.90	48744.0
174.90	3588.0
175.90	46776.0
176.90	3513.0
177.70	154.0

Instrument :
MSVOA_V
ClientSampleId :
BFB374

m/z	Abundance
35.90	349.0
36.90	2025.0
38.00	1890.0
39.00	786.0
39.90	312.0
43.00	164.0
43.90	638.0
45.00	427.0
46.20	234.0
47.00	503.0
47.80	363.0
49.00	1839.0
50.00	8260.0
51.00	2438.0
52.00	182.0
52.80	153.0
54.90	144.0
55.90	794.0
56.90	1026.0
60.00	542.0
60.90	2286.0
62.00	2015.0
62.90	2091.0
63.90	439.0
65.00	576.0
67.00	161.0
67.90	4589.0
69.00	4058.0
70.00	452.0
72.10	344.0
73.00	2144.0
74.00	7204.0
75.00	22016.0
76.00	1811.0
77.00	370.0
77.90	259.0
78.80	1672.0
79.80	534.0
80.90	1739.0
81.90	392.0
86.90	2206.0
87.90	1887.0
90.90	297.0
91.90	1369.0
93.00	1740.0
94.00	5869.0
95.00	48552.0
96.00	3118.0
103.70	231.0
104.70	116.0
106.00	127.0
116.00	143.0
116.90	334.0
117.80	111.0
118.90	419.0
127.80	191.0
129.10	176.0
129.90	228.0
135.00	114.0
136.70	121.0
140.90	418.0
141.80	159.0
142.90	798.0
144.80	435.0
145.80	120.0
147.90	170.0
154.90	162.0
158.50	102.0
170.90	218.0
171.90	475.0
172.90	621.0
173.90	44656.0
174.90	3163.0
175.90	42856.0
176.90	3083.0
177.80	131.0

Instrument :
MSVOA_V
ClientSampleId :
BFB374