

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092223\
 Data File : VV032158.D
 Acq On : 22 Sep 2023 12:47
 Operator : SY/MD
 Sample : 04469-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYP6

Quant Time: Sep 23 01:25:15 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Sep 23 01:24:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	240276	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	232256	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	118212	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	73879	49.130	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	98.260%		
7) Chloroethane-d5	1.532	69	62111	47.118	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	94.240%		
11) 1,1-Dichloroethene-d2	2.060	65	31408	44.606	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	89.220%		
21) 2-Butanone-d5	3.786	46	114274	96.623	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	96.620%		
24) Chloroform-d	4.252	84	141764	43.132	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	86.260%		
26) 1,2-Dichloroethane-d4	4.944	65	88717	40.673	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	81.340%		
32) Benzene-d6	4.963	84	288722	45.557	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	91.120%		
36) 1,2-Dichloropropane-d6	5.989	67	97358	47.728	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	95.460%		
41) Toluene-d8	7.246	98	258909	44.338	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	88.680%		
43) trans-1,3-Dichloroprop...	7.555	79	41024	38.802	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	77.600%		
47) 2-Hexanone-d5	8.027	63	69324	110.881	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	110.880%		
56) 1,1,2,2-Tetrachloroeth...	10.156	84	122584	46.504	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	93.000%		
66) 1,2-Dichlorobenzene-d4	11.564	152	101737	47.211	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	94.420%		
Target Compounds					Qvalue	
13) Acetone	2.114	43	12361	11.743	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092223\
Data File : VV032158.D
Acq On : 22 Sep 2023 12:47
Operator : SY/MD
Sample : 04469-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYP6

Quant Time: Sep 23 01:25:15 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Sep 23 01:24:00 2023
Response via : Initial Calibration

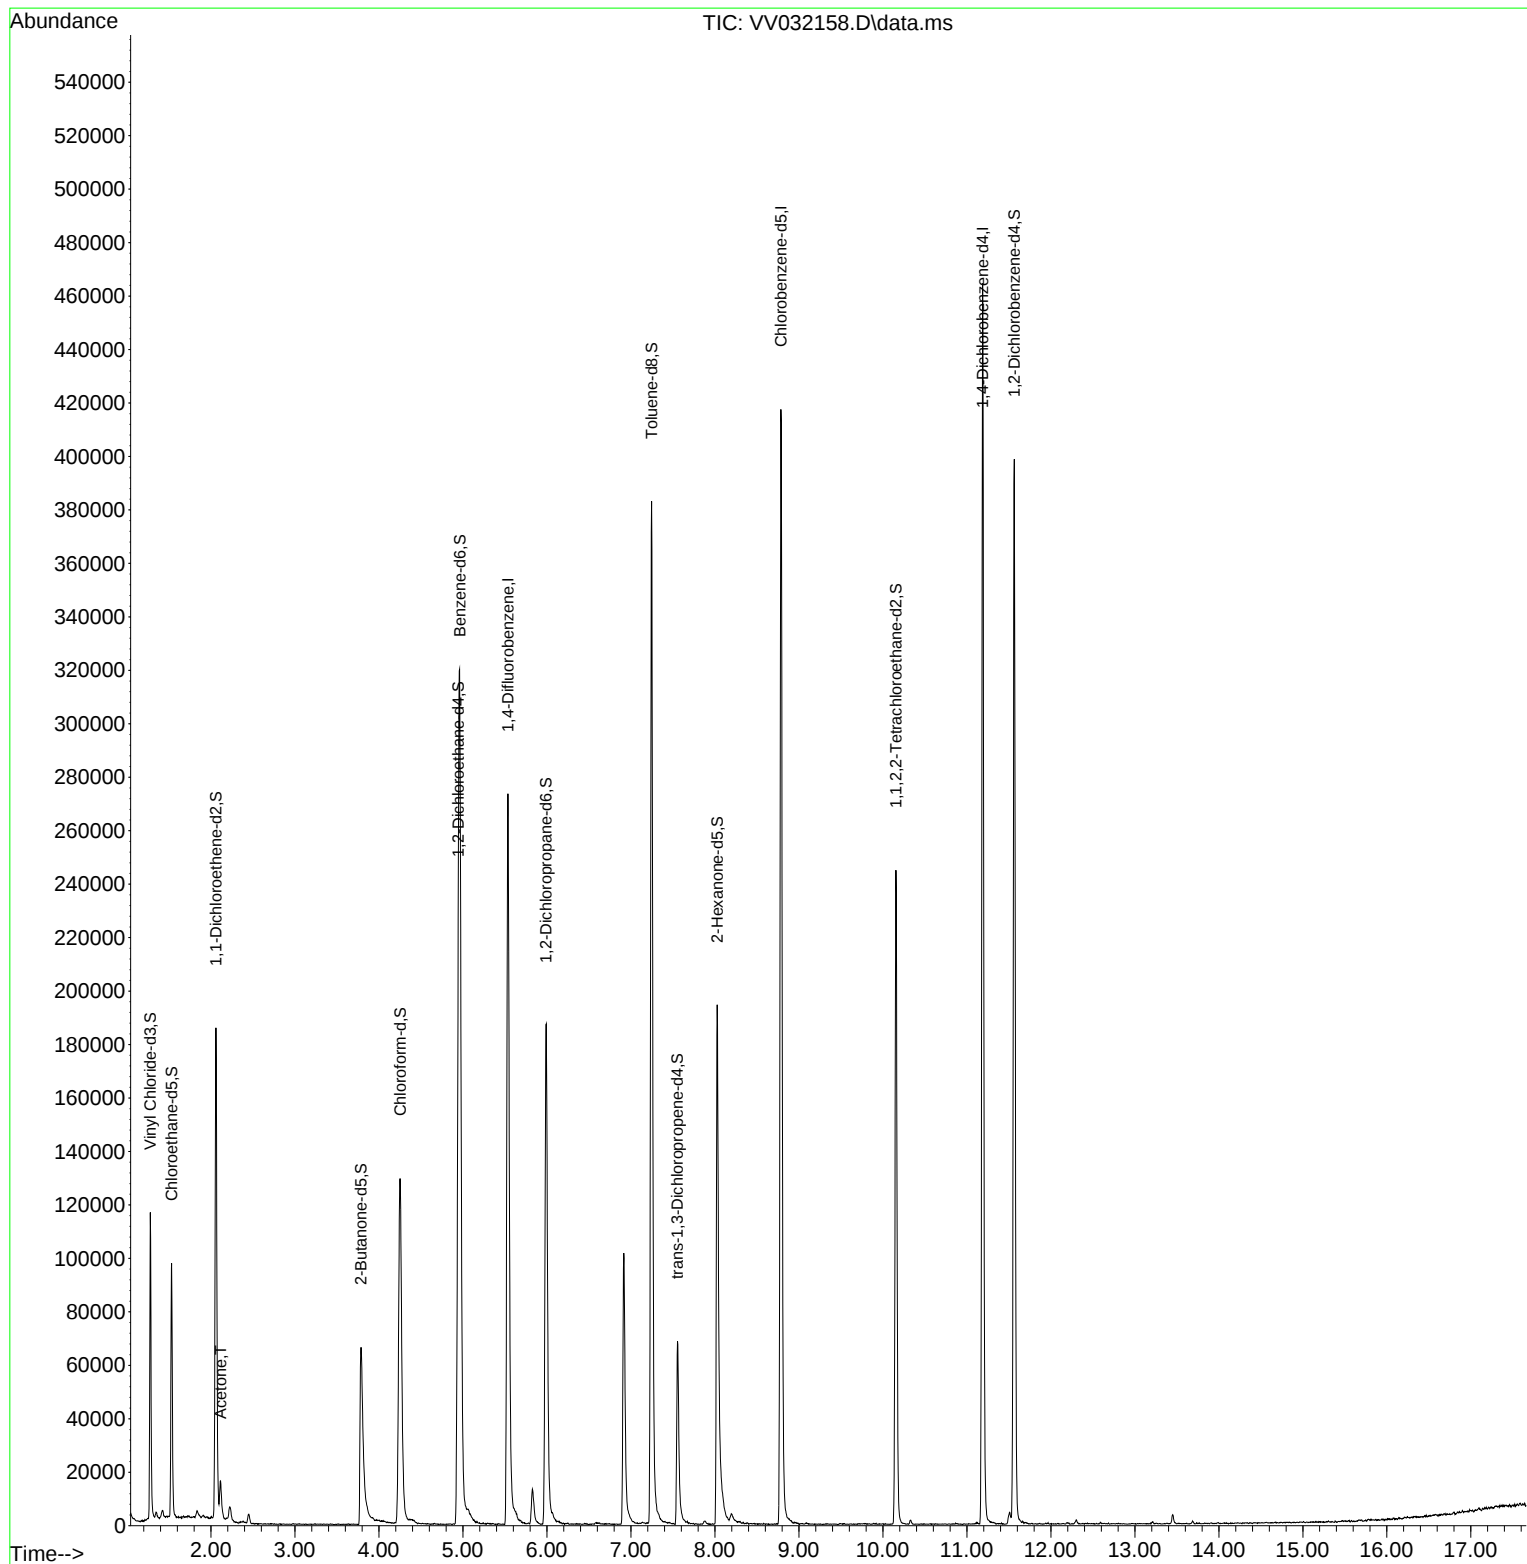

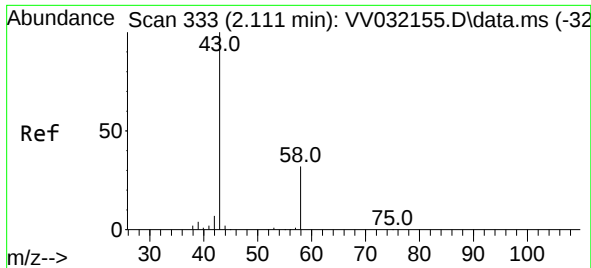

#13
 Acetone
 Concen: 11.743 ug/L
 RT: 2.114 min Scan# 31
 Delta R.T. 0.003 min
 Lab File: VV032158.D
 Acq: 22 Sep 2023 12:47

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYP6

Tgt Ion: 43 Resp: 12361
 Ion Ratio Lower Upper
 43 100
 58 34.5 0.0 61.0

