

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092223\
 Data File : VV032158.D
 Acq On : 22 Sep 2023 12:47
 Operator : SY/MD
 Sample : 04469-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYP6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV032158.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	90	rBV	114565	120544	14.20%	1.792%
2	1.532	146	153	170	rVB	95098	113648	13.39%	1.689%
3	2.060	308	317	328	rBV	182204	261249	30.78%	3.883%
4	2.449	431	438	448	rVB3	3540	5822	0.69%	0.087%
5	2.526	461	462	464	rBV3	240	112	0.01%	0.002%
6	2.574	474	477	479	rBV	217	145	0.02%	0.002%
7	2.754	530	533	537	rVB2	211	110	0.01%	0.002%
8	2.863	560	567	573	rBV2	175	262	0.03%	0.004%
9	2.970	597	600	601	rBV	261	97	0.01%	0.001%
10	3.034	617	620	623	rBV2	168	124	0.01%	0.002%
11	3.050	623	625	628	rVB	273	140	0.02%	0.002%
12	3.124	645	648	651	rBV	191	127	0.01%	0.002%
13	3.240	681	684	687	rVB	240	130	0.02%	0.002%
14	3.339	711	715	717	rBV	138	103	0.01%	0.002%
15	3.426	738	742	744	rVB	213	129	0.02%	0.002%
16	3.484	756	760	763	rBV	122	91	0.01%	0.001%
17	3.635	800	807	809	rBV	290	205	0.02%	0.003%
18	3.786	845	854	895	rBV	66331	187592	22.10%	2.788%
19	4.252	983	999	1030	rBV	128827	340262	40.09%	5.058%
20	4.632	1113	1117	1120	rBV2	246	187	0.02%	0.003%
21	4.651	1120	1123	1124	rBV	296	148	0.02%	0.002%
22	4.703	1136	1139	1141	rVB2	222	96	0.01%	0.001%
23	4.809	1170	1172	1176	rBV2	150	96	0.01%	0.001%
24	4.892	1192	1198	1200	rBV3	208	234	0.03%	0.003%
25	4.960	1200	1219	1245	rBV2	319876	848704	100.00%	12.615%
26	5.269	1313	1315	1318	rVB2	342	173	0.02%	0.003%
27	5.291	1318	1322	1323	rBV2	424	266	0.03%	0.004%
28	5.416	1358	1361	1362	rBV	314	135	0.02%	0.002%
29	5.535	1385	1398	1419	rBV	273353	562064	66.23%	8.354%
30	5.828	1479	1489	1509	rBV3	13046	28699	3.38%	0.427%
31	5.941	1521	1524	1526	rBV	197	133	0.02%	0.002%
32	5.992	1526	1540	1560	rBV	187246	393348	46.35%	5.847%
33	6.355	1650	1653	1656	rBV2	396	235	0.03%	0.003%
34	6.394	1661	1665	1669	rVB2	244	235	0.03%	0.003%
35	6.429	1673	1676	1679	rBV	123	95	0.01%	0.001%
36	6.445	1679	1681	1685	rBV2	266	175	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092223\
 Data File : VV032158.D
 Acq On : 22 Sep 2023 12:47
 Operator : SY/MD
 Sample : 04469-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYP6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	6.481	1690	1692	1696	rVB3	303	163	0.02%	0.002%
38	6.516	1700	1703	1706	rVB2	214	127	0.01%	0.002%
39	6.535	1706	1709	1711	rBV	193	145	0.02%	0.002%
40	6.577	1718	1722	1724	rBV3	580	492	0.06%	0.007%
41	6.703	1758	1761	1764	rVB2	309	144	0.02%	0.002%
42	6.719	1764	1766	1767	rBV	223	92	0.01%	0.001%
43	6.776	1783	1784	1789	rVB2	226	110	0.01%	0.002%
44	6.799	1789	1791	1793	rBV2	290	111	0.01%	0.002%
45	6.860	1804	1810	1811	rBV2	122	97	0.01%	0.001%
46	6.915	1816	1827	1861	rBV	101398	197137	23.23%	2.930%
47	7.194	1909	1914	1916	rBV3	500	401	0.05%	0.006%
48	7.246	1919	1930	1972	rVV	382307	688419	81.11%	10.233%
49	7.555	2017	2026	2056	rBV	68532	128383	15.13%	1.908%
50	7.770	2089	2093	2098	rBV4	335	319	0.04%	0.005%
51	7.834	2110	2113	2115	rBV	207	116	0.01%	0.002%
52	7.883	2118	2128	2133	rBV5	1216	2207	0.26%	0.033%
53	7.940	2143	2146	2149	rVB2	287	144	0.02%	0.002%
54	7.969	2152	2155	2160	rVB2	242	177	0.02%	0.003%
55	8.027	2164	2173	2217	rBV	194168	386296	45.52%	5.742%
56	8.487	2314	2316	2322	rBV3	217	215	0.03%	0.003%
57	8.526	2326	2328	2332	rVB3	244	178	0.02%	0.003%
58	8.609	2352	2354	2358	rBV2	258	190	0.02%	0.003%
59	8.635	2360	2362	2364	rVB2	337	158	0.02%	0.002%
60	8.657	2364	2369	2371	rBV2	162	132	0.02%	0.002%
61	8.715	2384	2387	2389	rVB	266	130	0.02%	0.002%
62	8.738	2391	2394	2396	rBV	307	194	0.02%	0.003%
63	8.786	2396	2409	2433	rBV	417083	699835	82.46%	10.402%
64	9.024	2478	2483	2484	rBV2	351	318	0.04%	0.005%
65	9.230	2545	2547	2550	rBV2	154	91	0.01%	0.001%
66	9.252	2552	2554	2559	rVV2	195	108	0.01%	0.002%
67	9.342	2579	2582	2585	rVB	164	110	0.01%	0.002%
68	9.487	2623	2627	2630	rBV3	380	333	0.04%	0.005%
69	9.526	2637	2639	2640	rBV	240	103	0.01%	0.002%
70	9.654	2677	2679	2682	rVB	252	129	0.02%	0.002%
71	9.680	2682	2687	2691	rBV2	165	141	0.02%	0.002%
72	9.706	2692	2695	2697	rBV	311	181	0.02%	0.003%
73	9.718	2697	2699	2703	rVB	219	123	0.01%	0.002%
74	9.789	2719	2721	2724	rBV2	194	96	0.01%	0.001%
75	9.889	2750	2752	2757	rVB3	383	306	0.04%	0.005%
76	9.918	2758	2761	2766	rVB2	374	216	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092223\
 Data File : VV032158.D
 Acq On : 22 Sep 2023 12:47
 Operator : SY/MD
 Sample : 04469-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYP6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	9.963	2772	2775	2779	rBV	230	161	0.02%	0.002%
78	10.034	2795	2797	2802	rVB	273	127	0.01%	0.002%
79	10.156	2823	2835	2859	rBV	244531	390810	46.05%	5.809%
80	10.326	2882	2888	2897	rBV5	1546	2284	0.27%	0.034%
81	10.490	2936	2939	2943	rBV2	206	134	0.02%	0.002%
82	10.622	2978	2980	2984	rBV2	316	194	0.02%	0.003%
83	10.783	3026	3030	3036	rBV2	174	220	0.03%	0.003%
84	10.834	3043	3046	3048	rBV2	202	118	0.01%	0.002%
85	10.866	3053	3056	3059	rBV2	377	232	0.03%	0.003%
86	10.940	3076	3079	3082	rVB2	177	112	0.01%	0.002%
87	10.966	3082	3087	3088	rBV	298	212	0.02%	0.003%
88	11.111	3128	3132	3133	rBV2	546	302	0.04%	0.004%
89	11.188	3145	3156	3177	rBV	464046	715351	84.29%	10.633%
90	11.358	3206	3209	3210	rBV2	223	152	0.02%	0.002%
91	11.413	3224	3226	3229	rVB3	437	220	0.03%	0.003%
92	11.509	3245	3256	3261	rBV4	4394	7978	0.94%	0.119%
93	11.564	3262	3273	3291	rVB	397044	627546	73.94%	9.328%
94	11.847	3358	3361	3362	rBV	232	107	0.01%	0.002%
95	12.085	3430	3435	3437	rBV2	340	273	0.03%	0.004%
96	12.194	3464	3469	3471	rBV4	463	485	0.06%	0.007%
97	12.304	3495	3503	3507	rBV5	1465	1879	0.22%	0.028%
98	12.564	3582	3584	3588	rBV	177	92	0.01%	0.001%
99	12.587	3589	3591	3596	rVV3	485	394	0.05%	0.006%
100	13.451	3855	3860	3868	rVB3	3078	4103	0.48%	0.061%




Sum of corrected areas: 6727768

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092223\
Data File : VV032158.D
Acq On : 22 Sep 2023 12:47
Operator : SY/MD
Sample : 04469-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYP6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

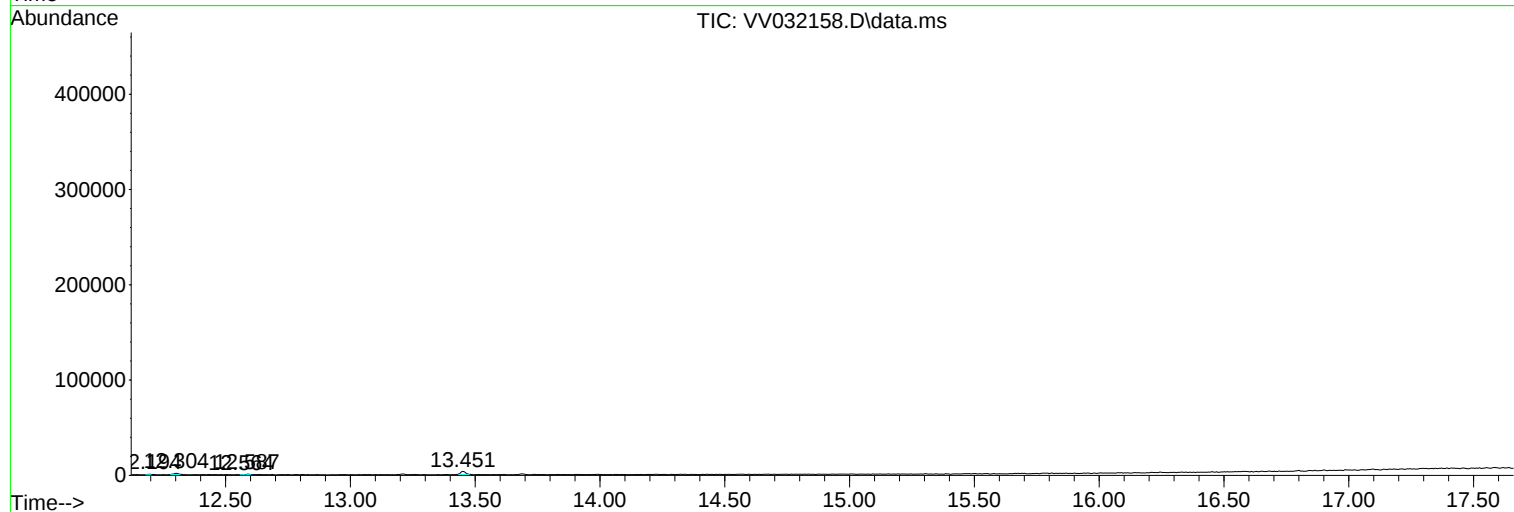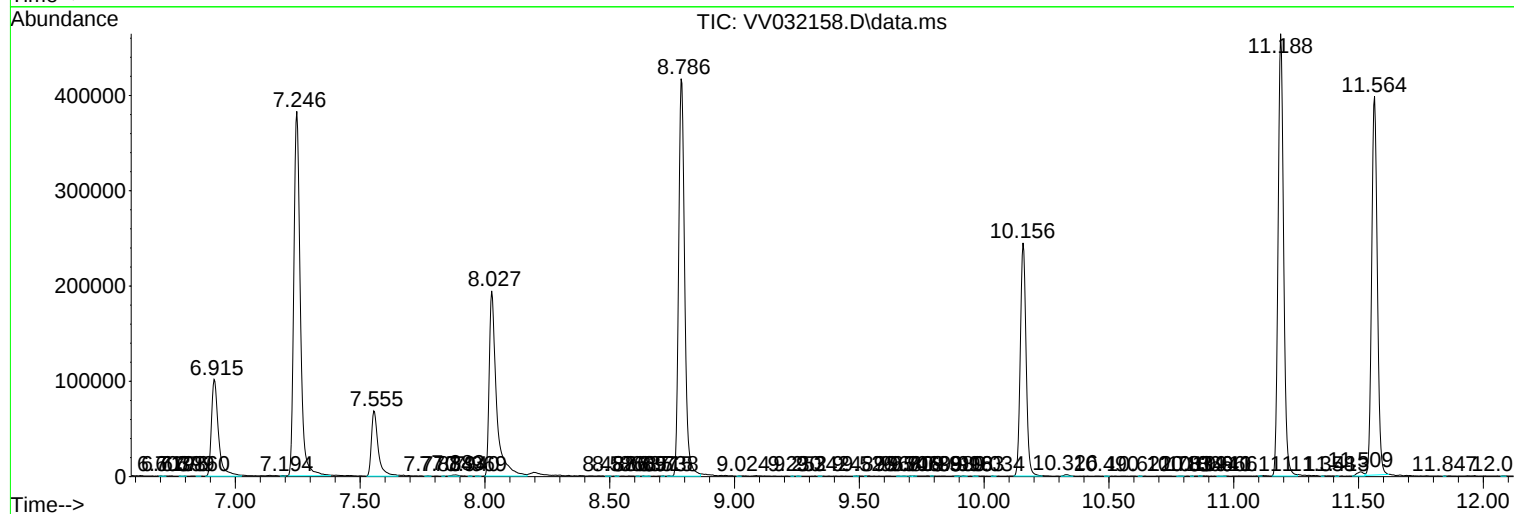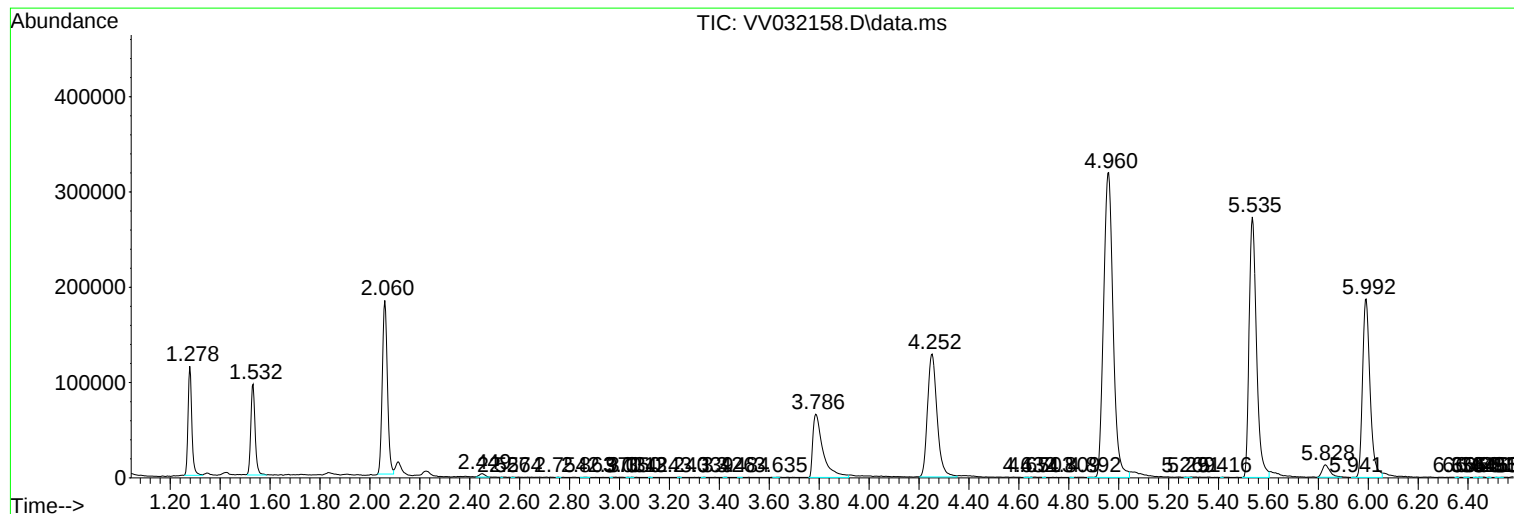

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092223\
Data File : VV032158.D
Acq On : 22 Sep 2023 12:47
Operator : SY/MD
Sample : 04469-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYP6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092223\
Data File : VV032158.D
Acq On : 22 Sep 2023 12:47
Operator : SY/MD
Sample : 04469-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZY6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc