

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092223\
 Data File : VV032159.D
 Acq On : 22 Sep 2023 13:11
 Operator : SY/MD
 Sample : 04469-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYS1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV032159.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	50	55	62	rBV2	3218	4031	0.51%	0.062%
2	1.278	67	74	91	rVV	106836	113211	14.25%	1.747%
3	1.532	145	153	165	rBV	90071	106722	13.43%	1.647%
4	2.060	306	317	328	rBV	169888	246510	31.03%	3.804%
5	2.224	362	368	387	rVB	8420	16107	2.03%	0.249%
6	2.323	397	399	400	rBV2	321	147	0.02%	0.002%
7	2.442	432	436	441	rBV3	917	1143	0.14%	0.018%
8	2.571	472	476	479	rVV3	498	319	0.04%	0.005%
9	2.587	479	481	485	rVB2	375	216	0.03%	0.003%
10	2.677	507	509	513	rVB2	215	130	0.02%	0.002%
11	2.783	538	542	544	rBV2	189	170	0.02%	0.003%
12	2.986	601	605	608	rBV	208	154	0.02%	0.002%
13	3.002	608	610	614	rVV2	212	172	0.02%	0.003%
14	3.198	667	671	677	rVB2	318	237	0.03%	0.004%
15	3.494	760	763	766	rBV3	203	166	0.02%	0.003%
16	3.789	845	855	886	rBV	63543	176236	22.18%	2.720%
17	4.252	982	999	1024	rBV	120839	309319	38.93%	4.773%
18	4.552	1090	1092	1095	rBV3	294	231	0.03%	0.004%
19	4.568	1095	1097	1101	rVB2	355	228	0.03%	0.004%
20	4.629	1114	1116	1118	rBV	291	134	0.02%	0.002%
21	4.690	1129	1135	1136	rBV2	225	164	0.02%	0.003%
22	4.741	1148	1151	1155	rBV4	222	187	0.02%	0.003%
23	4.793	1161	1167	1171	rVB3	318	345	0.04%	0.005%
24	4.960	1202	1219	1246	rBV2	301019	794531	100.00%	12.261%
25	5.156	1278	1280	1283	rVB3	318	200	0.03%	0.003%
26	5.362	1340	1344	1348	rBV3	351	243	0.03%	0.004%
27	5.381	1348	1350	1355	rVB2	210	149	0.02%	0.002%
28	5.490	1381	1384	1386	rBV2	364	187	0.02%	0.003%
29	5.535	1386	1398	1426	rBV	277900	578773	72.84%	8.932%
30	5.828	1479	1489	1511	rBV2	13507	30194	3.80%	0.466%
31	5.992	1526	1540	1565	rBV	173793	371463	46.75%	5.733%
32	6.243	1614	1618	1621	rBV	227	173	0.02%	0.003%
33	6.281	1624	1630	1635	rVB3	370	414	0.05%	0.006%
34	6.391	1660	1664	1669	rBV2	403	339	0.04%	0.005%
35	6.497	1693	1697	1698	rBV2	213	140	0.02%	0.002%
36	6.915	1817	1827	1855	rBV2	91692	181695	22.87%	2.804%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092223\
 Data File : VV032159.D
 Acq On : 22 Sep 2023 13:11
 Operator : SY/MD
 Sample : 04469-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYS1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	7.104	1884	1886	1890	rVB2	263	167	0.02%	0.003%
38	7.140	1894	1897	1903	rVV2	518	458	0.06%	0.007%
39	7.191	1910	1913	1916	rVB2	289	166	0.02%	0.003%
40	7.246	1918	1930	1965	rBV	352931	634248	79.83%	9.788%
41	7.558	2016	2027	2046	rBV	62561	114520	14.41%	1.767%
42	7.770	2091	2093	2096	rBV2	241	148	0.02%	0.002%
43	7.802	2102	2103	2108	rBV	178	154	0.02%	0.002%
44	7.879	2118	2127	2135	rBV3	1604	2284	0.29%	0.035%
45	7.931	2141	2143	2148	rBV2	235	220	0.03%	0.003%
46	8.027	2164	2173	2212	rBV	189754	377148	47.47%	5.820%
47	8.194	2218	2225	2242	rVB6	3952	8753	1.10%	0.135%
48	8.368	2277	2279	2282	rVB3	422	235	0.03%	0.004%
49	8.384	2282	2284	2290	rVB3	286	196	0.02%	0.003%
50	8.426	2290	2297	2305	rBV4	533	707	0.09%	0.011%
51	8.471	2309	2311	2317	rVB	428	320	0.04%	0.005%
52	8.513	2321	2324	2325	rBV	322	150	0.02%	0.002%
53	8.558	2335	2338	2343	rVB2	285	226	0.03%	0.003%
54	8.580	2343	2345	2348	rBV	271	130	0.02%	0.002%
55	8.786	2397	2409	2437	rBV	423592	710743	89.45%	10.968%
56	9.014	2477	2480	2486	rBV2	415	480	0.06%	0.007%
57	9.146	2515	2521	2525	rBV	245	246	0.03%	0.004%
58	9.384	2588	2595	2600	rBV	182	162	0.02%	0.003%
59	9.879	2745	2749	2753	rBV3	179	148	0.02%	0.002%
60	9.905	2754	2757	2761	rBV2	241	136	0.02%	0.002%
61	9.982	2779	2781	2786	rVB	199	142	0.02%	0.002%
62	10.066	2804	2807	2810	rBV2	234	146	0.02%	0.002%
63	10.156	2822	2835	2855	rBV	232273	367669	46.27%	5.674%
64	10.272	2869	2871	2875	rBV	226	150	0.02%	0.002%
65	10.326	2883	2888	2898	rVB3	1629	2225	0.28%	0.034%
66	10.561	2959	2961	2965	rVB2	221	167	0.02%	0.003%
67	10.905	3062	3068	3070	rBV6	742	946	0.12%	0.015%
68	11.066	3116	3118	3120	rVB	360	151	0.02%	0.002%
69	11.111	3130	3132	3134	rVV2	348	144	0.02%	0.002%
70	11.136	3138	3140	3143	rVB	308	129	0.02%	0.002%
71	11.188	3144	3156	3179	rBV	468766	721036	90.75%	11.127%
72	11.342	3202	3204	3209	rVB3	263	238	0.03%	0.004%
73	11.500	3246	3253	3262	rBV4	4323	8812	1.11%	0.136%
74	11.564	3262	3273	3296	rVB	363215	578442	72.80%	8.927%
75	11.709	3314	3318	3322	rBV4	487	429	0.05%	0.007%
76	11.757	3330	3333	3335	rBV2	196	155	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092223\
 Data File : VV032159.D
 Acq On : 22 Sep 2023 13:11
 Operator : SY/MD
 Sample : 04469-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYS1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	11.770	3335	3337	3343	rVB2	312	201	0.03%	0.003%
78	11.796	3343	3345	3346	rBV2	506	162	0.02%	0.003%
79	11.886	3371	3373	3374	rBV2	306	135	0.02%	0.002%
80	11.921	3381	3384	3385	rBV2	220	131	0.02%	0.002%
81	12.059	3424	3427	3433	rVB2	377	267	0.03%	0.004%
82	12.120	3439	3446	3451	rVB3	519	621	0.08%	0.010%
83	12.169	3458	3461	3464	rBV2	171	143	0.02%	0.002%
84	12.204	3468	3472	3473	rVV2	294	212	0.03%	0.003%
85	12.300	3495	3502	3508	rBV3	2621	3551	0.45%	0.055%
86	12.435	3541	3544	3549	rBV	244	201	0.03%	0.003%
87	12.574	3585	3587	3589	rBV2	263	173	0.02%	0.003%
88	12.587	3589	3591	3594	rBV2	207	143	0.02%	0.002%
89	12.898	3686	3688	3694	rVB2	343	264	0.03%	0.004%
90	12.931	3694	3698	3702	rBV2	245	295	0.04%	0.005%
91	13.413	3846	3848	3852	rVB2	280	186	0.02%	0.003%
92	13.451	3852	3860	3867	rBV3	2518	3370	0.42%	0.052%
93	13.542	3884	3888	3890	rBV	195	186	0.02%	0.003%
94	13.615	3909	3911	3915	rVB3	276	184	0.02%	0.003%
95	13.763	3953	3957	3959	rBV2	196	164	0.02%	0.003%
96	13.979	4021	4024	4027	rBV	349	319	0.04%	0.005%
97	14.149	4073	4077	4080	rBV2	270	281	0.04%	0.004%
98	14.368	4140	4145	4147	rBV	303	262	0.03%	0.004%
99	14.747	4261	4263	4265	rBV2	345	190	0.02%	0.003%
100	15.705	4558	4561	4563	rBV	710	400	0.05%	0.006%




Sum of corrected areas: 6479947

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092223\
Data File : VV032159.D
Acq On : 22 Sep 2023 13:11
Operator : SY/MD
Sample : 04469-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYS1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

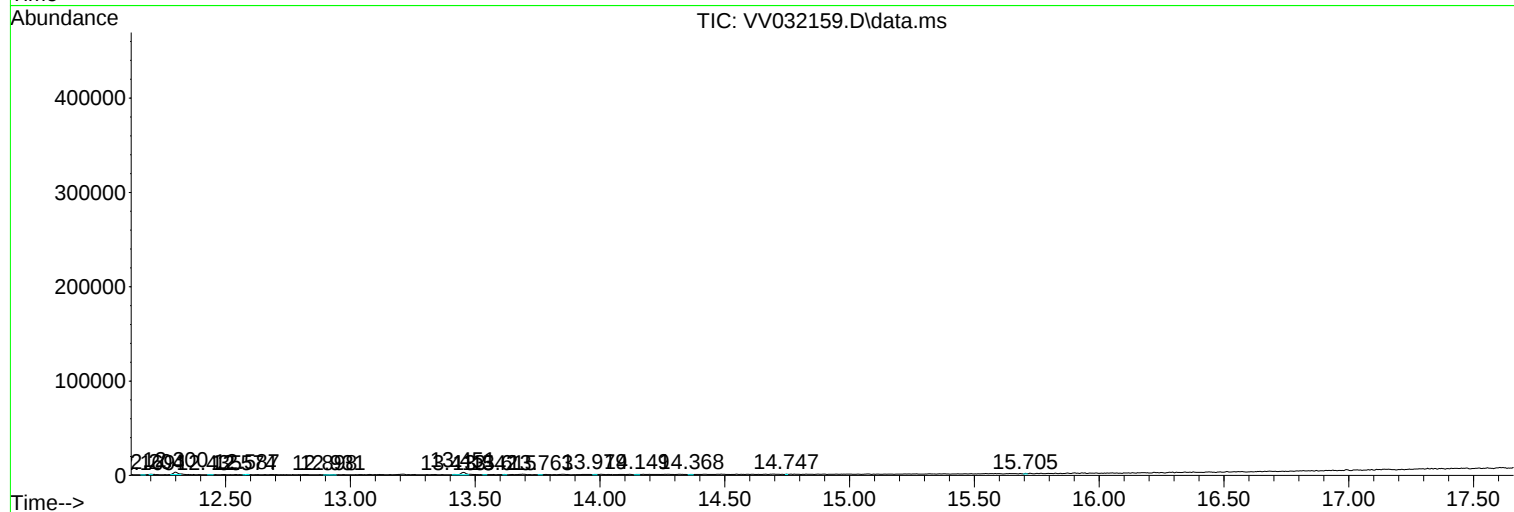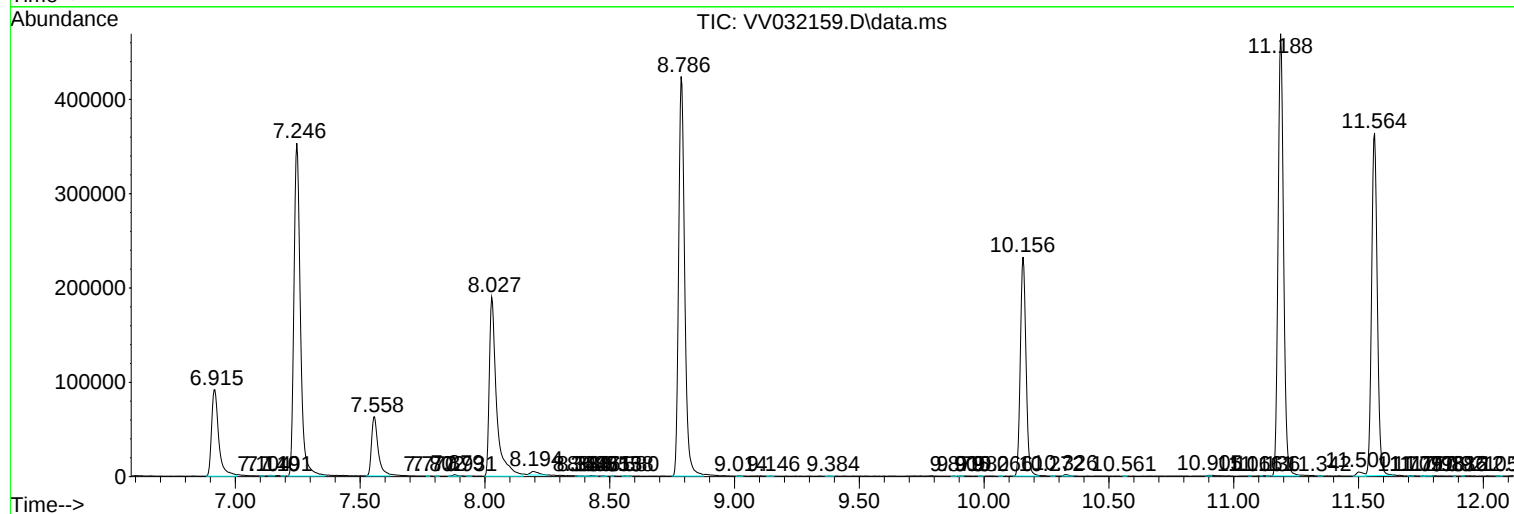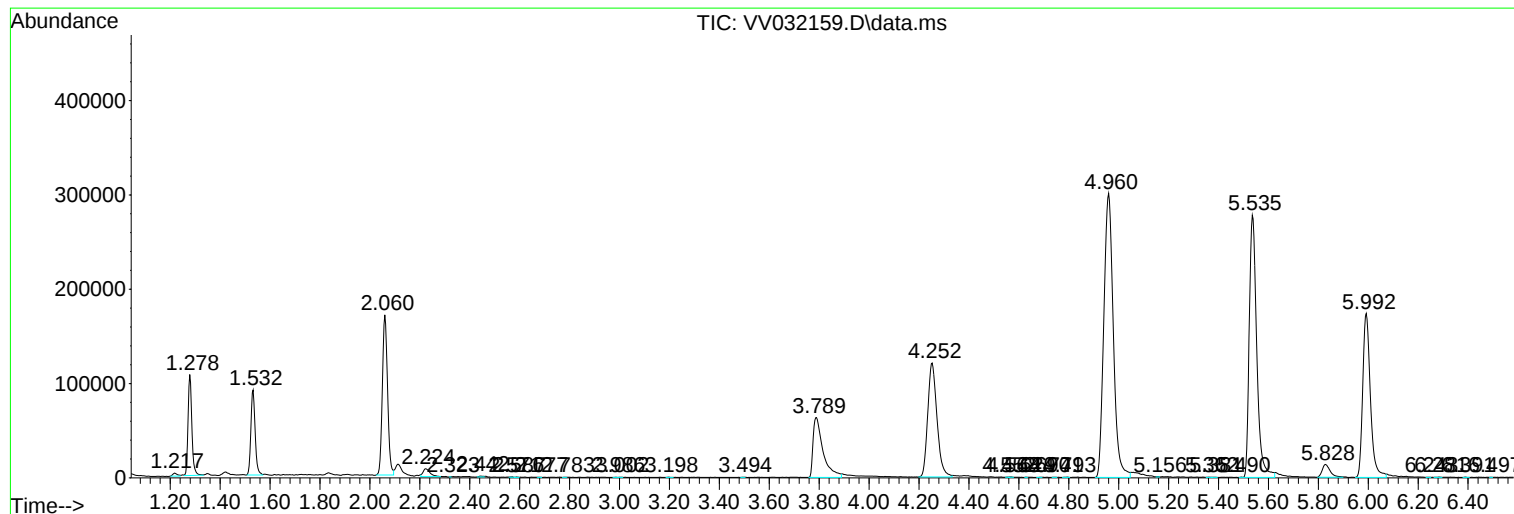

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092223\
Data File : VV032159.D
Acq On : 22 Sep 2023 13:11
Operator : SY/MD
Sample : 04469-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYS1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092223\
Data File : VV032159.D
Acq On : 22 Sep 2023 13:11
Operator : SY/MD
Sample : 04469-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYS1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc