


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092223\
Data File : VV032153.D
Acq On : 22 Sep 2023 08:56
Operator : SY/MD
Sample : BFB215
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB215

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Title : VOC Analysis
Last Update : Sat Sep 23 01:24:00 2023

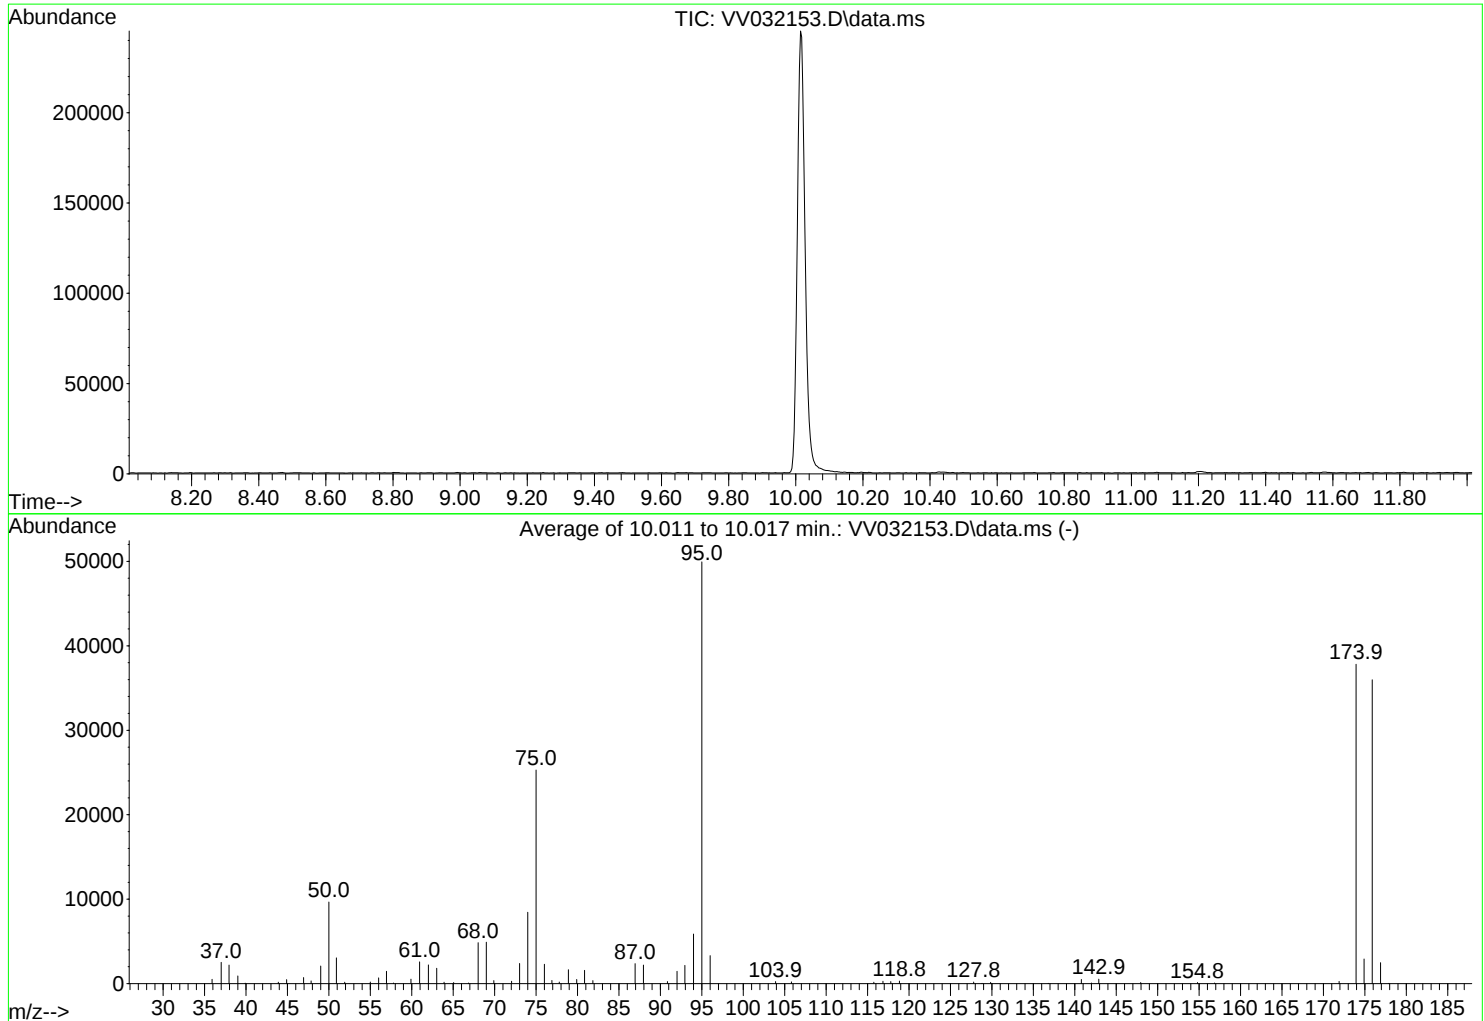

AutoFind: Scans 2790, 2791, 2792; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	9673	PASS
75	95	30	80	50.6	25288	PASS
95	95	100	100	100.0	49944	PASS
96	95	5	9	6.6	3321	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	75.7	37811	PASS
175	174	5	9	7.7	2919	PASS
176	174	95	105	95.1	35968	PASS
177	176	5	10	6.9	2487	PASS

m/z	Abundance
40.00	173.0
44.00	439.0

Instrument :
MSVOA_V
ClientSampleId :
BFB215

m/z	Abundance
35.90	492.0
37.00	2472.0
37.90	2164.0
39.00	924.0
39.90	204.0
43.90	614.0
44.90	480.0
47.00	759.0
47.90	321.0
49.00	1991.0
50.00	9442.0
50.90	2994.0
51.90	168.0
55.00	199.0
56.00	731.0
57.00	1358.0
59.90	563.0
60.90	2492.0
62.00	2052.0
63.00	1783.0
63.90	167.0
65.00	118.0
66.80	100.0
68.00	4739.0
69.00	4757.0
69.90	369.0
72.10	299.0
73.00	2257.0
74.00	8013.0
75.00	24152.0
76.00	2148.0
76.90	429.0
77.80	178.0
78.90	1583.0
79.90	468.0
80.90	1539.0
81.90	343.0
86.90	2277.0
87.90	2124.0
90.90	227.0
92.00	1367.0
93.00	2071.0
94.00	5693.0
95.00	47048.0
96.00	3182.0
103.90	205.0
105.80	223.0
115.70	175.0
116.90	287.0
117.80	224.0
118.80	284.0
127.80	170.0
129.90	144.0
140.80	436.0
142.00	111.0
142.90	475.0
147.90	117.0
154.80	139.0
171.90	282.0
173.90	35248.0
174.90	2772.0
175.90	33224.0
176.90	2354.0

Instrument :
MSVOA_V
ClientSampleId :
BFB215

m/z	Abundance
35.90	534.0
37.00	2598.0
38.00	2254.0
39.00	925.0
39.90	227.0
43.90	609.0
44.90	487.0
47.00	727.0
47.80	327.0
49.00	2149.0
50.00	9974.0
50.90	3167.0
51.90	174.0
55.00	189.0
56.00	687.0
57.00	1515.0
57.80	107.0
59.90	544.0
61.00	2680.0
62.00	2271.0
63.00	1861.0
63.90	184.0
65.10	130.0
68.00	5021.0
69.00	5075.0
69.90	359.0
72.10	303.0
73.00	2457.0
74.00	8725.0
75.00	26144.0
76.00	2392.0
76.90	378.0
77.90	178.0
78.90	1726.0
79.90	504.0
80.80	1624.0
81.90	355.0
87.00	2473.0
88.00	2327.0
90.80	250.0
92.00	1506.0
93.00	2224.0
94.00	6059.0
95.00	51664.0
96.00	3482.0
103.90	254.0
105.80	224.0
115.70	177.0
116.80	301.0
117.80	261.0
118.80	308.0
127.80	213.0
129.90	159.0
136.80	102.0
140.80	533.0
142.00	114.0
142.90	534.0
147.90	128.0
154.80	141.0
156.80	103.0
171.90	263.0
173.90	39104.0
174.90	2993.0
175.90	37104.0
176.90	2559.0
177.90	101.0

Instrument :
MSVOA_V
ClientSampleId :
BFB215

m/z	Abundance
35.90	516.0
37.00	2485.0
38.00	2161.0
39.00	908.0
39.90	232.0
43.80	600.0
44.90	456.0
46.90	659.0
47.80	330.0
49.00	2103.0
50.00	9604.0
50.90	2995.0
51.90	156.0
55.00	166.0
56.00	630.0
56.90	1523.0
57.80	111.0
59.90	504.0
61.00	2564.0
62.00	2340.0
63.00	1803.0
63.90	167.0
65.10	137.0
66.90	134.0
68.00	4824.0
69.00	4895.0
69.90	367.0
72.00	271.0
73.00	2433.0
74.00	8600.0
75.00	25568.0
76.00	2347.0
76.90	326.0
77.70	208.0
78.90	1658.0
79.90	492.0
80.80	1565.0
81.80	376.0
87.00	2334.0
88.00	2159.0
90.80	252.0
92.00	1505.0
92.90	2175.0
94.00	5889.0
95.00	51120.0
96.00	3298.0
103.90	264.0
105.80	202.0
115.80	180.0
116.80	298.0
117.80	263.0
118.90	301.0
127.80	215.0
128.80	102.0
129.80	164.0
140.80	537.0
142.90	579.0
148.00	137.0
154.80	146.0
156.90	101.0
171.90	228.0
174.00	39080.0
174.90	2992.0
175.90	37576.0
176.90	2549.0

Instrument :
MSVOA_V
ClientSampleId :
BFB215