
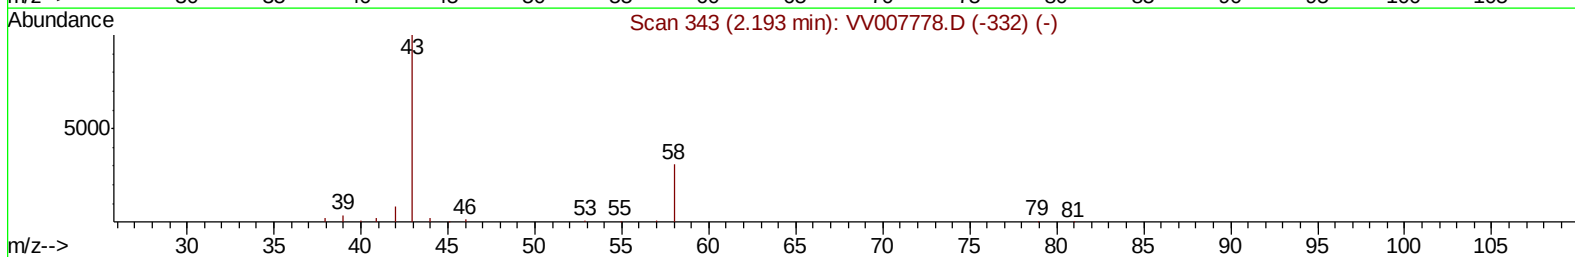
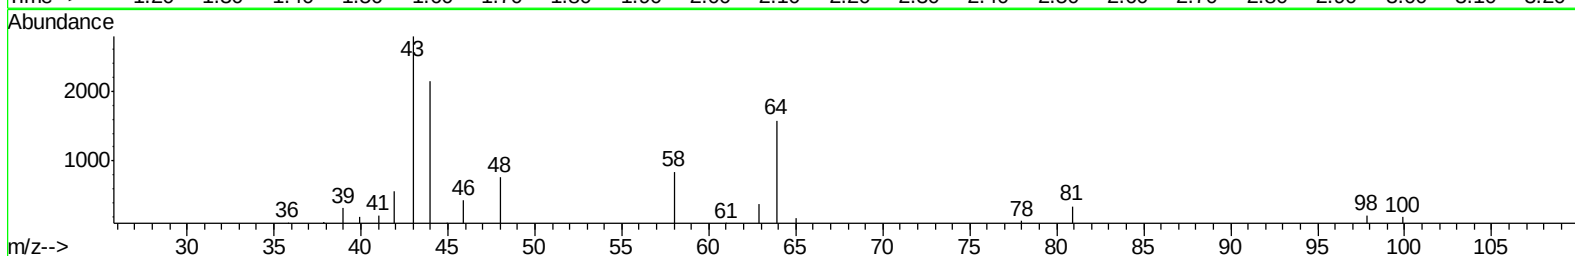


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV092318\
Data File : VV007793.D
Acq On : 23 Sep 2018 17:12
Operator : SY/MD
Sample : J5014-08
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 71 Sample Multiplier: 1

Quant Time: Sep 24 07:22:44 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092318WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Sep 24 07:19:48 2018
Response via : Initial Calibration

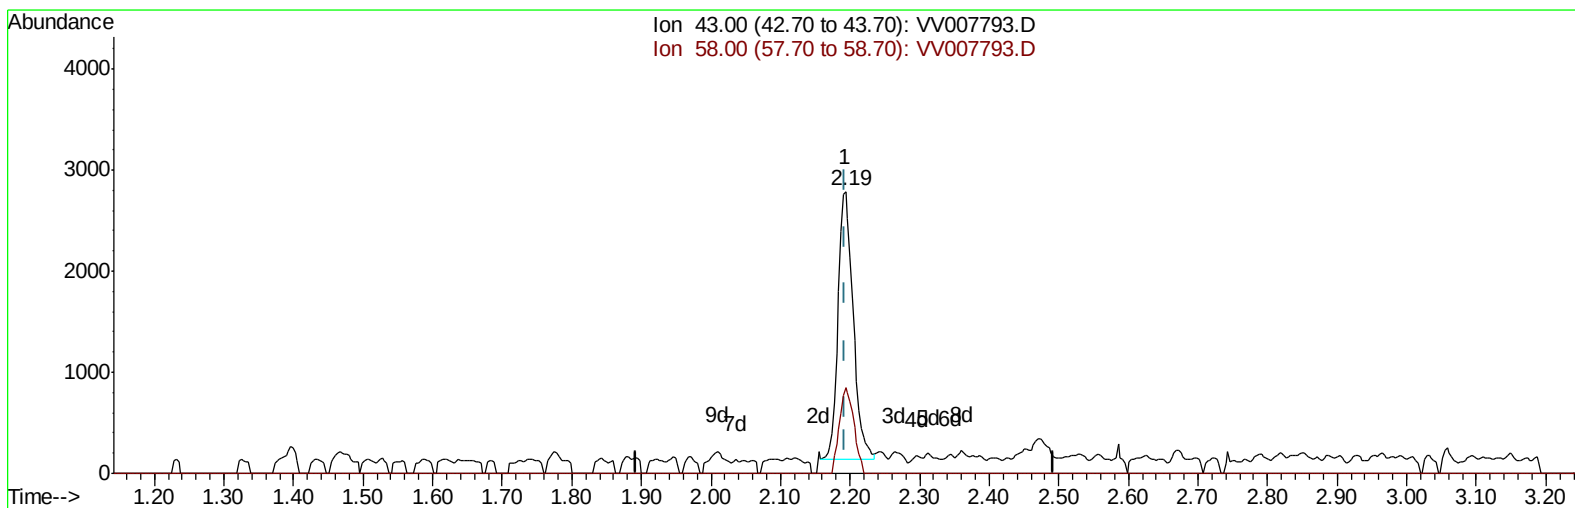

TIC: VV007793.D

(13) Acetone (T)

2.193min (+0.000) 5.36ug/L m

response 3987

Ion	Exp%	Act%
43.00	100	100
58.00	32.60	30.57
0.00	0.00	0.00
0.00	0.00	0.00