

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092318\
 Data File : VV007766.D
 Acq On : 23 Sep 2018 05:05
 Operator : SY/MD
 Sample : J5013-06
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C08T8

Quant Time: Sep 24 06:52:11 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092318WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Sep 24 05:16:03 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	180143	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	174566	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	91153	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	45900	46.88	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	93.76%
7) Chloroethane-d5	1.59	69	46241	51.97	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	103.94%
11) 1,1-Dichloroethene-d2	2.14	63	86969	37.68	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	75.36%
21) 2-Butanone-d5	3.95	46	59163	91.50	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	91.50%
24) Chloroform-d	4.41	84	97092	46.32	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.64%
26) 1,2-Dichloroethane-d4	5.09	65	66166	49.49	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.98%
32) Benzene-d6	5.11	84	199511	49.72	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.44%
36) 1,2-Dichloropropane-d6	6.13	67	59030	49.82	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	99.64%
41) Toluene-d8	7.36	98	205505	49.01	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	98.02%
43) trans-1,3-Dichloropropene-	7.67	79	25160	42.12	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	84.24%
47) 2-Hexanone-d5	8.14	63	46534	89.18	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	89.18%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	86229	46.62	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	93.24%
64) 1,2-Dichlorobenzene-d4	11.68	152	92739	49.46	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	98.92%


Target Compounds					Ovalue
13) Acetone	2.19	43	2783	4.078 ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV092318\
Data File : VV007766.D
Acq On : 23 Sep 2018 05:05
Operator : SY/MD
Sample : J5013-06
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C08T8

Quant Time: Sep 24 06:52:11 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092318WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Sep 24 05:16:03 2018
Response via : Initial Calibration

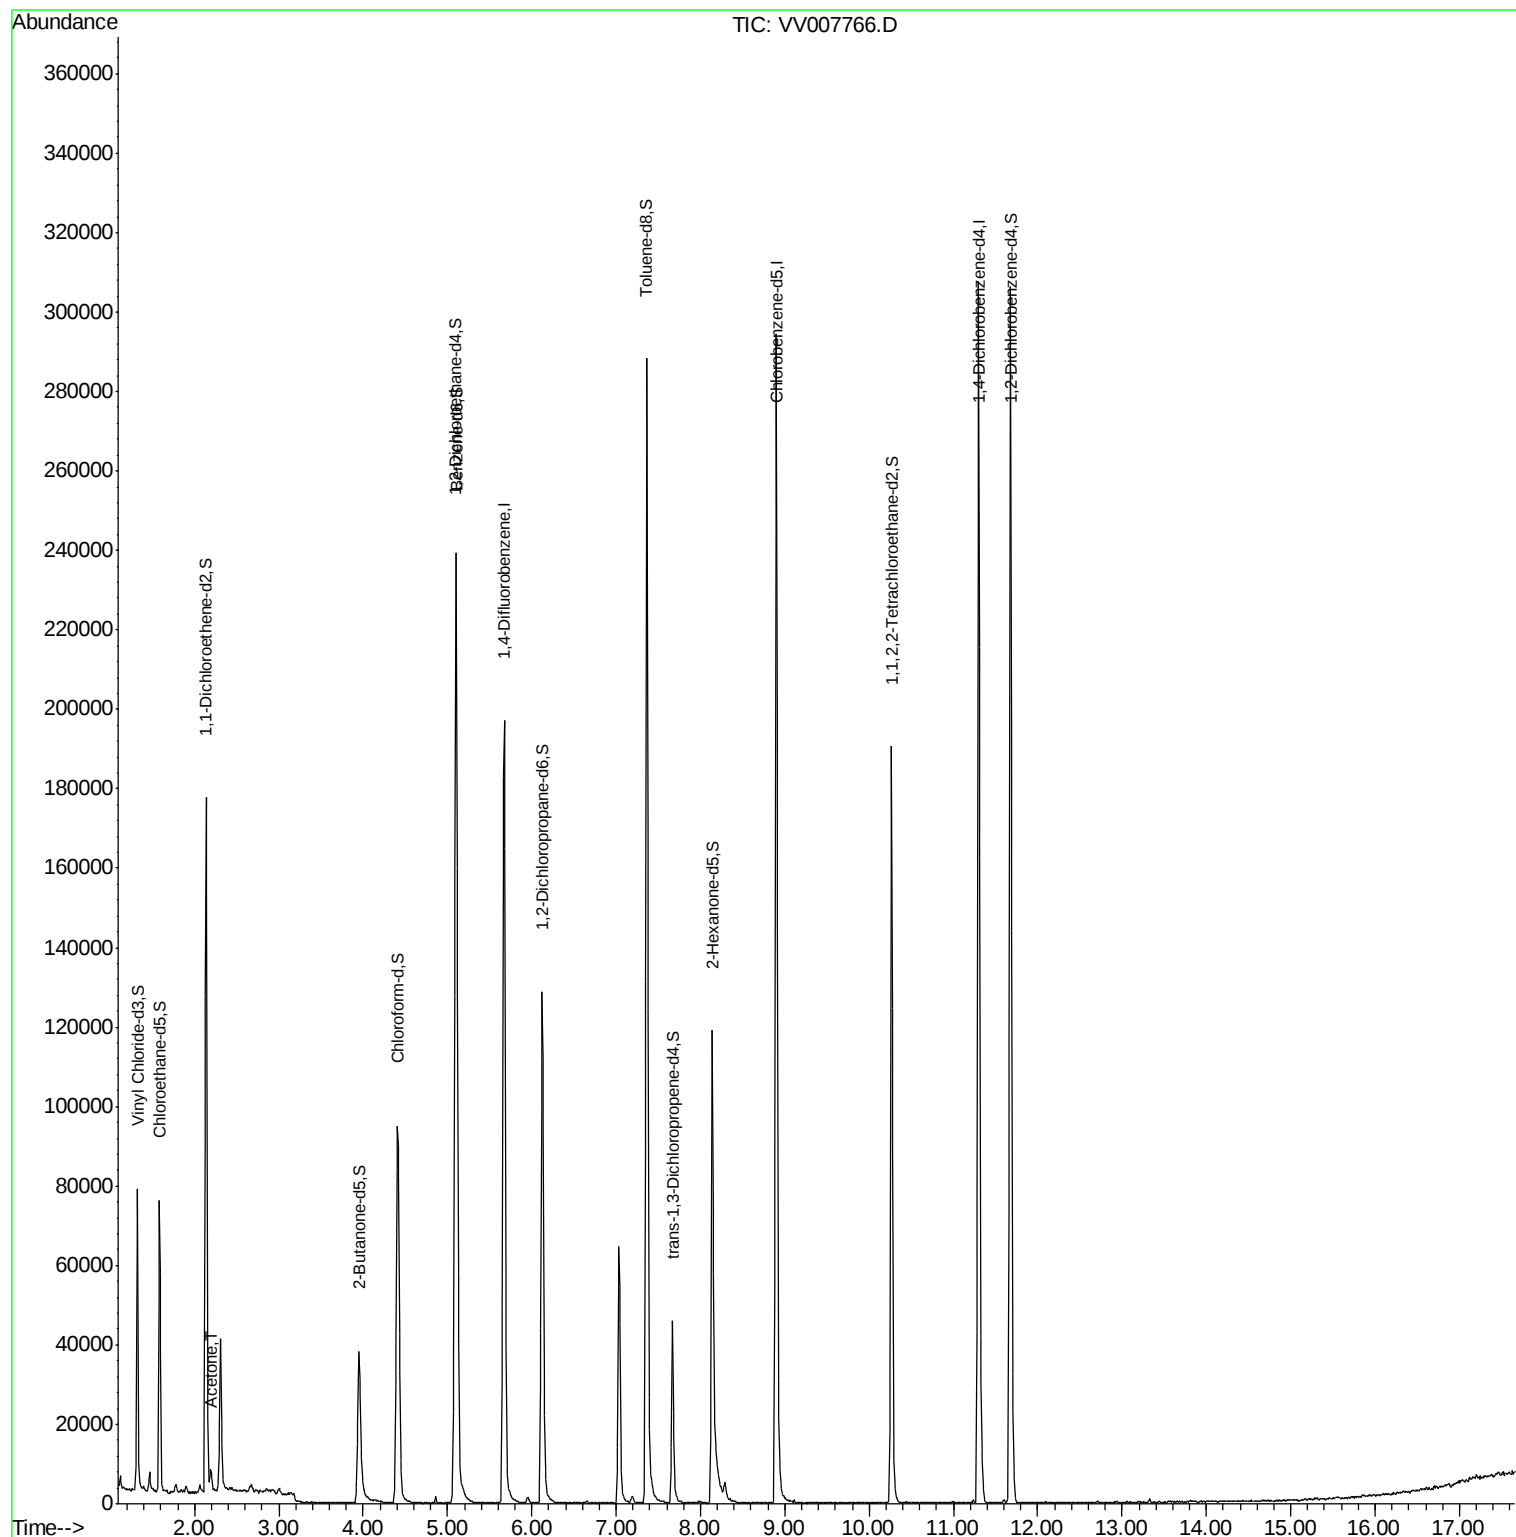

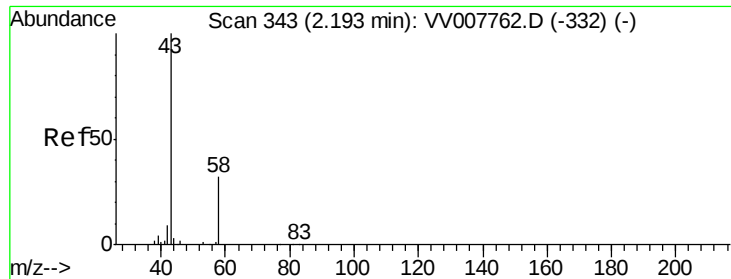

#13

Acetone

Concen: 4.078 ug/L

RT: 2.19 min Scan# 342

Delta R.T. -0.00 min

Lab File: VV007766.D

Acq: 23 Sep 2018 05:05

Instrument :
MSVOA_V
ClientSampleId :
C08T8

Tot Ion: 43 Resp: 2783

Ion Ratio Lower Upper

43 100

58 32.7 0.0 65.2

