

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092318\
 Data File : VV007785.D
 Acq On : 23 Sep 2018 13:53
 Operator : SY/MD
 Sample : J5014-10
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E8JC4

Quant Time: Sep 24 07:51:10 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092318WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Sep 24 07:19:48 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	173976	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	166685	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	87584	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	36146	38.23	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	76.46%
7) Chloroethane-d5	1.59	69	37827	44.02	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	88.04%
11) 1,1-Dichloroethene-d2	2.14	63	74799	33.55	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	67.10%
21) 2-Butanone-d5	3.95	46	60414	96.74	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	96.74%
24) Chloroform-d	4.41	84	89491	44.21	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.42%
26) 1,2-Dichloroethane-d4	5.09	65	60705	47.01	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.02%
32) Benzene-d6	5.11	84	176806	46.15	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.30%
36) 1,2-Dichloropropane-d6	6.13	67	53459	47.25	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	94.50%
41) Toluene-d8	7.36	98	184722	46.14	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.28%
43) trans-1,3-Dichloropropene-	7.67	79	24209	42.44	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	84.88%
47) 2-Hexanone-d5	8.14	63	42743	85.79	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	85.79%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	79934	45.26	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	90.52%
64) 1,2-Dichlorobenzene-d4	11.68	152	86662	48.10	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	96.20%


Target Compounds					Ovalue
13) Acetone	2.19	43	4123	6.256 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV092318\
Data File : VV007785.D
Acq On : 23 Sep 2018 13:53
Operator : SY/MD
Sample : J5014-10
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 63 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E8JC4

Quant Time: Sep 24 07:51:10 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092318WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Sep 24 07:19:48 2018
Response via : Initial Calibration

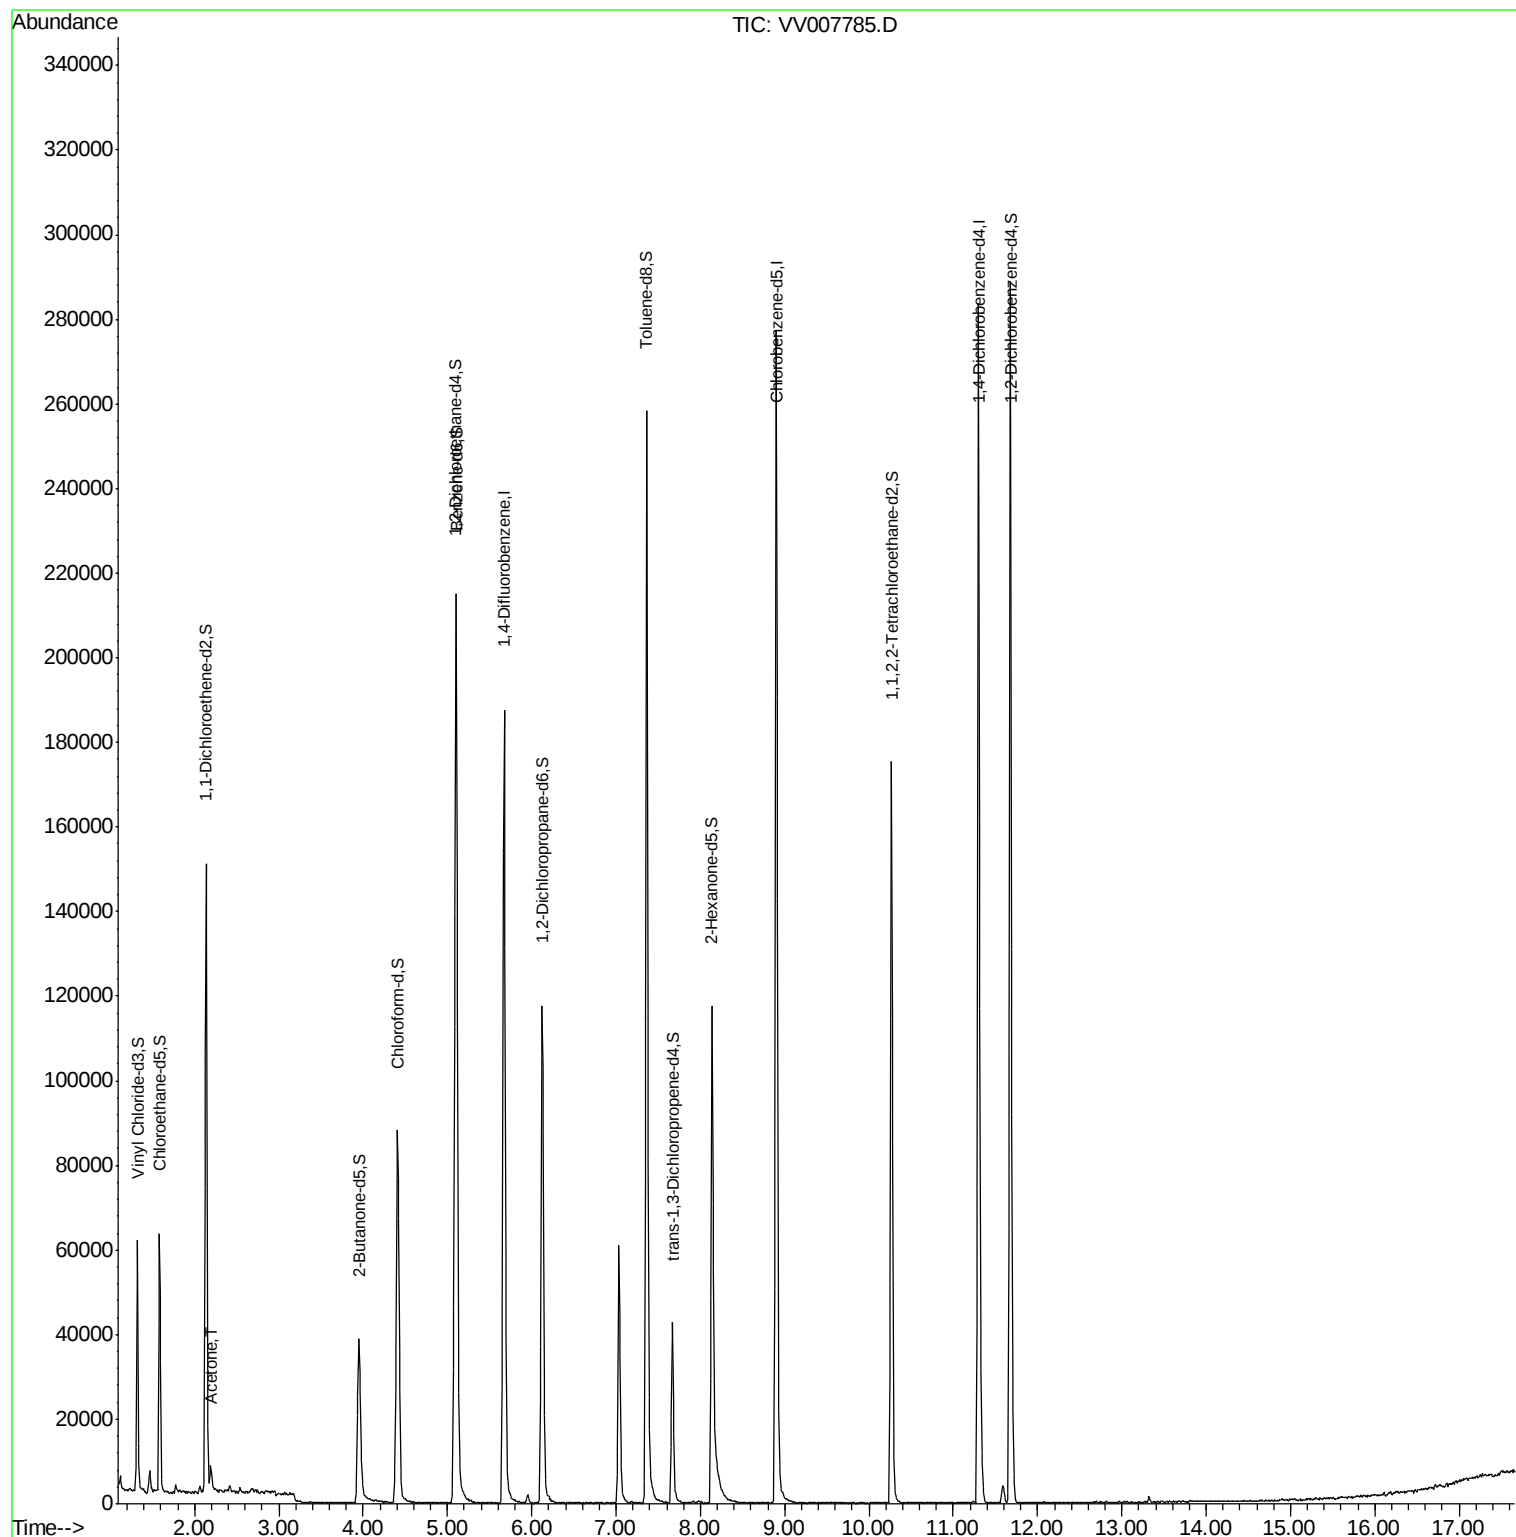

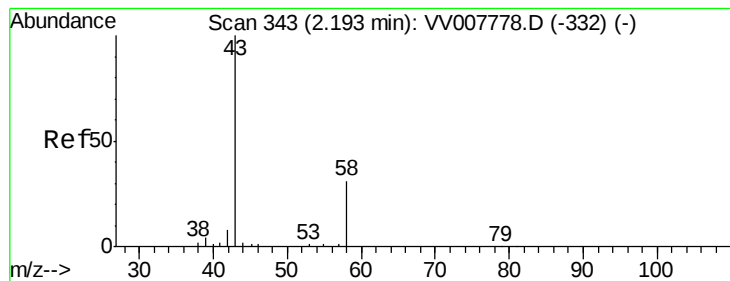

#13

Acetone

Concen: 6.256 ug/L

RT: 2.19 min Scan# 343

Delta R.T. 0.00 min

Lab File: VV007785.D

Acq: 23 Sep 2018 13:53

Instrument :
MSVOA_V
ClientSampleId :
E8JC4

Tot Ion: 43 Resp: 4123

Ion Ratio Lower Upper

43 100

58 30.4 0.0 65.2

