

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092318\
 Data File : VV007763.D
 Acq On : 23 Sep 2018 03:50
 Operator : SY/MD
 Sample : VV0923WBL02
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK63

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092318WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.322	65	72	89	rVB	79322	85057	13.77%	1.679%
2	1.585	147	154	165	rVB	76108	86829	14.06%	1.714%
3	2.135	315	325	340	rBV	182319	266087	43.08%	5.253%
4	3.296	683	686	692	rVB	257	174	0.03%	0.003%
5	3.376	708	711	717	rVB	197	177	0.03%	0.003%
6	3.576	770	773	778	rBV	148	107	0.02%	0.002%
7	3.949	876	889	916	rBV	41459	112733	18.25%	2.226%
8	4.412	1015	1033	1057	rBV	98408	247466	40.07%	4.886%
9	4.588	1085	1088	1090	rBV2	147	107	0.02%	0.002%
10	4.984	1208	1211	1217	rVB	98	92	0.01%	0.002%
11	5.032	1221	1226	1229	rBV	141	136	0.02%	0.003%
12	5.103	1229	1248	1272	rBV2	253193	617633	100.00%	12.194%
13	5.453	1352	1357	1360	rBV2	166	129	0.02%	0.003%
14	5.469	1360	1362	1369	rVB	221	156	0.03%	0.003%
15	5.508	1369	1374	1376	rBV	108	97	0.02%	0.002%
16	5.672	1409	1425	1456	rBV	198980	404960	65.57%	7.995%
17	5.849	1478	1480	1487	rVB2	334	271	0.04%	0.005%
18	5.952	1505	1512	1520	rVB5	1224	1831	0.30%	0.036%
19	6.019	1529	1533	1538	rBV	101	100	0.02%	0.002%
20	6.125	1551	1566	1586	rBV	134131	276144	44.71%	5.452%
21	6.289	1615	1617	1623	rBV	188	167	0.03%	0.003%
22	6.646	1725	1728	1734	rBV3	392	350	0.06%	0.007%
23	6.910	1805	1810	1814	rVB	96	92	0.01%	0.002%
24	7.035	1837	1849	1874	rBV	67283	123885	20.06%	2.446%
25	7.170	1889	1891	1896	rVV2	314	270	0.04%	0.005%
26	7.202	1899	1901	1905	rVB	325	204	0.03%	0.004%
27	7.270	1919	1922	1927	rVB	241	128	0.02%	0.003%
28	7.366	1935	1952	1982	rBV	300961	549666	89.00%	10.852%
29	7.604	2024	2026	2032	rVB2	246	196	0.03%	0.004%
30	7.669	2034	2046	2067	rBV	47742	83238	13.48%	1.643%
31	7.858	2097	2105	2108	rVV	195	222	0.04%	0.004%
32	7.881	2108	2112	2118	rVB2	235	221	0.04%	0.004%
33	7.920	2120	2124	2126	rBV2	128	101	0.02%	0.002%
34	7.981	2140	2143	2148	rBV2	279	362	0.06%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092318\
 Data File : VV007763.D
 Acq On : 23 Sep 2018 03:50
 Operator : SY/MD
 Sample : VV0923WBL02
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK63

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092318WMA.M
 Title : VOC Analysis

35	8.022	2153	2156	2163	rVB3	491	570	0.09%	0.011%
36	8.055	2163	2166	2168	rBV2	154	93	0.02%	0.002%
37	8.077	2168	2173	2176	rVB	109	102	0.02%	0.002%
38	8.138	2181	2192	2236	rBV	125600	266919	43.22%	5.270%
39	8.569	2321	2326	2328	rBV	161	102	0.02%	0.002%
40	8.685	2354	2362	2364	rBV	73	102	0.02%	0.002%
41	8.730	2373	2376	2384	rVB	189	193	0.03%	0.004%
42	8.801	2392	2398	2399	rBV	168	118	0.02%	0.002%
43	8.900	2414	2429	2458	rBV	298703	508163	82.28%	10.033%
44	9.190	2509	2519	2524	rBV3	487	706	0.11%	0.014%
45	9.309	2551	2556	2559	rBV	146	117	0.02%	0.002%
46	9.582	2639	2641	2643	rBV	196	99	0.02%	0.002%
47	9.601	2643	2647	2651	rBV3	289	298	0.05%	0.006%
48	9.736	2684	2689	2691	rBV	117	104	0.02%	0.002%
49	9.868	2725	2730	2736	rBV	86	111	0.02%	0.002%
50	10.054	2785	2788	2795	rVB	93	111	0.02%	0.002%
51	10.267	2842	2854	2884	rVB	201847	328633	53.21%	6.488%
52	10.437	2904	2907	2909	rBV	174	100	0.02%	0.002%
53	10.479	2914	2920	2922	rBV	110	107	0.02%	0.002%
54	10.527	2931	2935	2938	rVB	188	96	0.02%	0.002%
55	10.559	2938	2945	2949	rBV	110	154	0.02%	0.003%
56	10.823	3022	3027	3033	rBV	146	156	0.03%	0.003%
57	10.942	3060	3064	3068	rBV	197	125	0.02%	0.002%
58	11.122	3111	3120	3123	rBV	117	120	0.02%	0.002%
59	11.196	3139	3143	3147	rVB	121	95	0.02%	0.002%
60	11.231	3147	3154	3162	rBV	1038	1459	0.24%	0.029%
61	11.299	3162	3175	3206	rVB	308221	529014	85.65%	10.444%
62	11.485	3229	3233	3235	rVV	234	179	0.03%	0.004%
63	11.675	3279	3292	3314	rBV	323381	555335	89.91%	10.964%
64	11.775	3321	3323	3326	rBV	151	114	0.02%	0.002%
65	11.800	3326	3331	3336	rVV2	160	164	0.03%	0.003%
66	11.874	3351	3354	3356	rBV2	170	110	0.02%	0.002%
67	11.903	3360	3363	3367	rBV	124	103	0.02%	0.002%
68	11.929	3367	3371	3375	rVB2	157	153	0.02%	0.003%
69	12.013	3391	3397	3398	rBV	177	145	0.02%	0.003%
70	12.090	3416	3421	3423	rBV2	151	109	0.02%	0.002%
71	12.116	3425	3429	3433	rBV	221	214	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092318\
 Data File : VV007763.D
 Acq On : 23 Sep 2018 03:50
 Operator : SY/MD
 Sample : VV0923WBL02
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK63

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092318WMA.M
 Title : VOC Analysis

72	12.164	3442	3444	3450	rBV2	175	154	0.02%	0.003%
73	12.318	3490	3492	3494	rBV2	152	109	0.02%	0.002%
74	12.357	3499	3504	3509	rVB2	239	321	0.05%	0.006%
75	12.469	3536	3539	3544	rVB	189	132	0.02%	0.003%
76	12.514	3550	3553	3557	rBV	186	188	0.03%	0.004%
77	12.566	3566	3569	3573	rVB2	247	187	0.03%	0.004%
78	12.614	3581	3584	3586	rBV2	134	117	0.02%	0.002%
79	12.701	3603	3611	3618	rBV3	1203	1713	0.28%	0.034%
80	12.759	3627	3629	3635	rVB	228	177	0.03%	0.003%
81	12.788	3635	3638	3642	rBV	110	106	0.02%	0.002%
82	12.855	3655	3659	3661	rBV2	218	178	0.03%	0.004%
83	12.874	3661	3665	3666	rBV	215	129	0.02%	0.003%
84	12.958	3685	3691	3694	rBV2	227	229	0.04%	0.005%
85	12.993	3694	3702	3705	rBV2	215	326	0.05%	0.006%
86	13.067	3722	3725	3726	rVV	193	100	0.02%	0.002%
87	13.254	3779	3783	3785	rBV	125	122	0.02%	0.002%
88	13.321	3796	3804	3814	rBV5	1788	2582	0.42%	0.051%
89	13.566	3872	3880	3888	rBV	509	826	0.13%	0.016%
90	13.717	3925	3927	3933	rBV2	186	169	0.03%	0.003%
91	13.781	3944	3947	3948	rBV	150	97	0.02%	0.002%
92	13.804	3948	3954	3963	rVB4	948	1365	0.22%	0.027%
93	13.868	3971	3974	3976	rBV	165	102	0.02%	0.002%
94	13.903	3982	3985	3989	rBV	232	160	0.03%	0.003%
95	14.347	4120	4123	4126	rBV	254	118	0.02%	0.002%
96	14.553	4185	4187	4190	rBV2	329	151	0.02%	0.003%
97	14.903	4294	4296	4298	rBV2	302	170	0.03%	0.003%
98	15.180	4379	4382	4387	rBV	361	254	0.04%	0.005%
99	15.459	4465	4469	4472	rBV2	620	539	0.09%	0.011%
100	15.707	4543	4546	4547	rBV	502	304	0.05%	0.006%


Sum of corrected areas: 5065106

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV092318\
Data File : VV007763.D
Acq On : 23 Sep 2018 03:50
Operator : SY/MD
Sample : VV0923WBL02
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK63

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092318WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

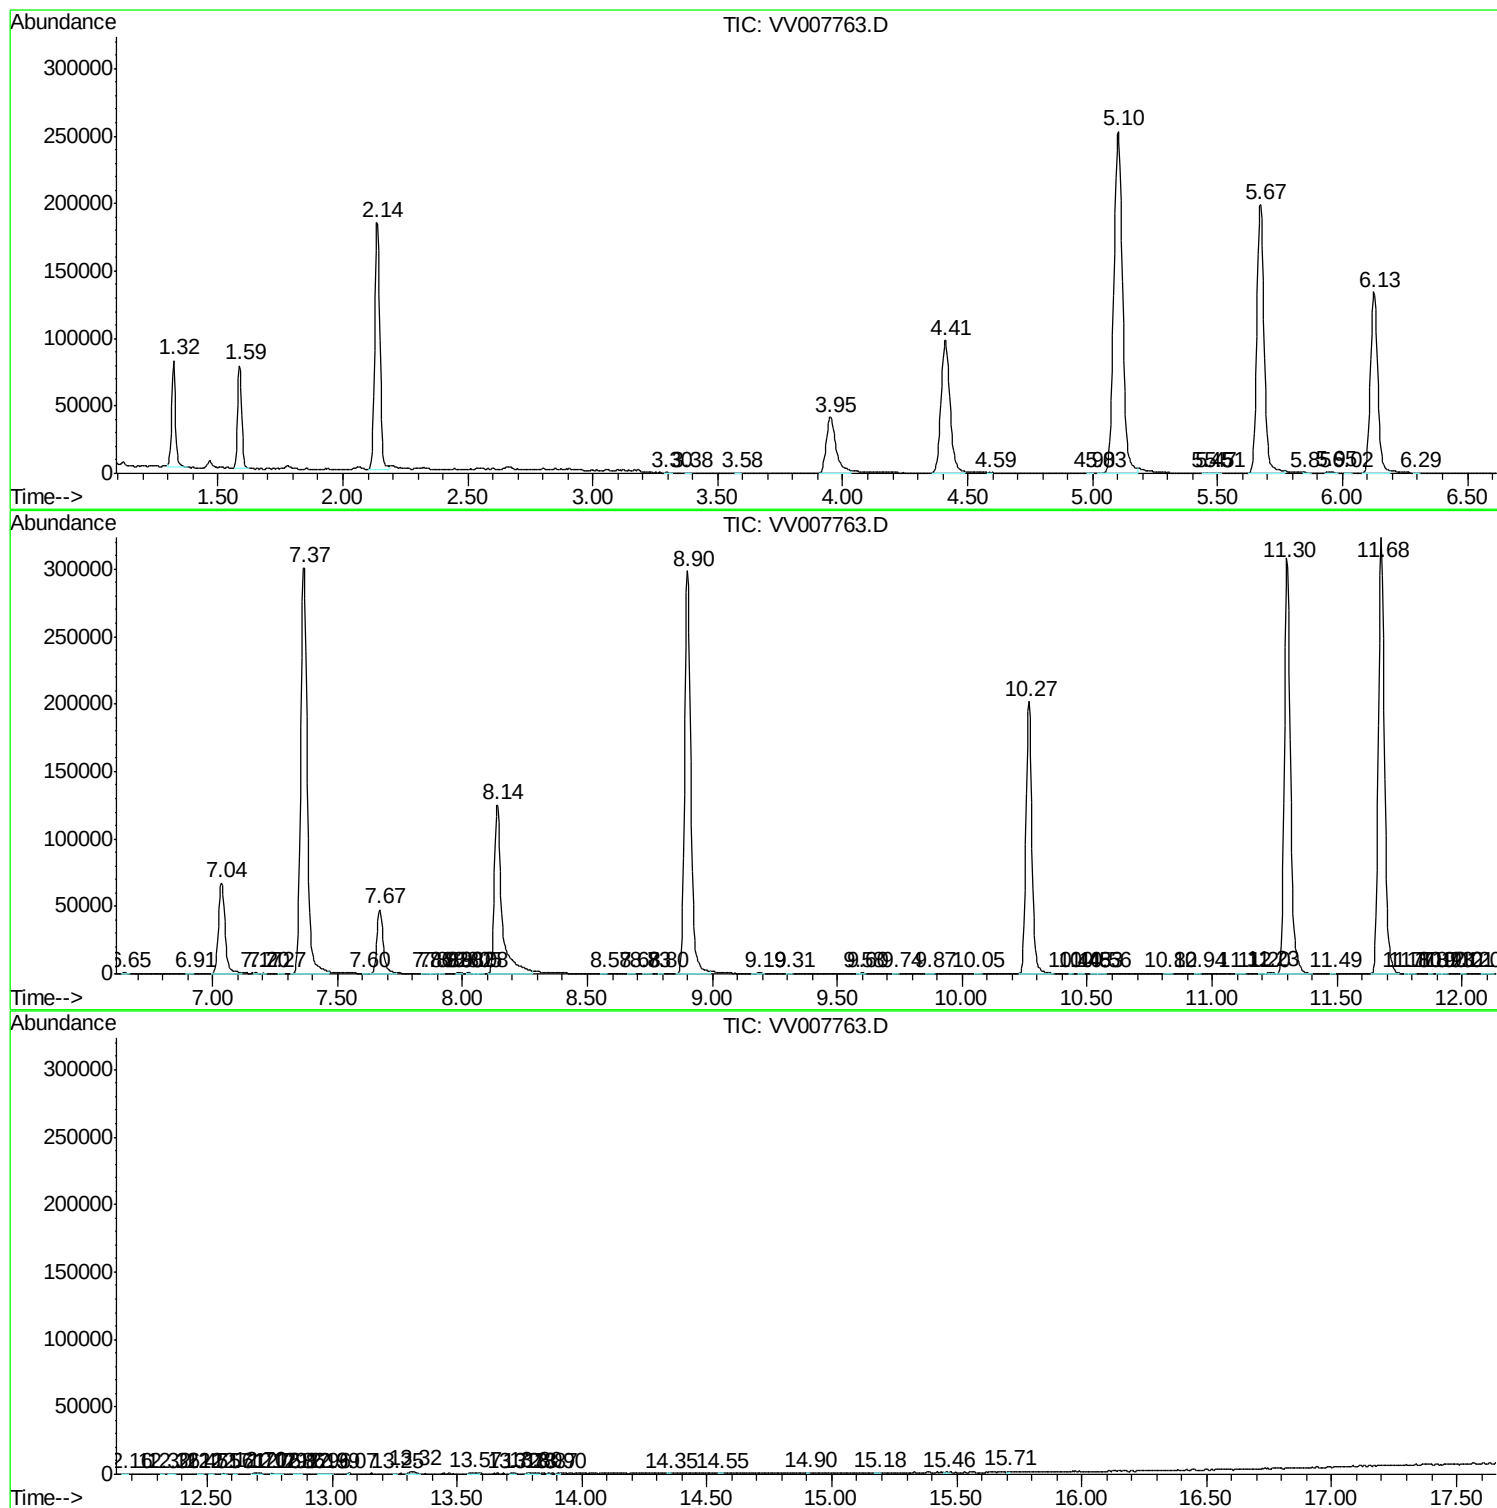

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV092318\
Data File : VV007763.D
Acq On : 23 Sep 2018 03:50
Operator : SY/MD
Sample : VV0923WBL02
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK63

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092318WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV092318\
Data File : VV007763.D
Acq On : 23 Sep 2018 03:50
Operator : SY/MD
Sample : VV0923WBL02
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK63

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092318WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc