

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092318\
 Data File : VV007764.D
 Acq On : 23 Sep 2018 04:15
 Operator : SY/MD
 Sample : J5013-04
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C08T2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092318WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.322	67	72	91	rVB	66878	68094	0.14%	0.126%
2	1.585	148	154	166	rVB	62782	71199	0.14%	0.132%
3	2.139	317	326	336	rBV	152425	214466	0.43%	0.397%
4	2.354	365	393	504	rBV2	16613443	49393087	100.00%	91.511%
5	4.412	1014	1033	1058	rBV	89348	217864	0.44%	0.404%
6	4.740	1132	1135	1137	rBV	70	48	0.00%	0.000%
7	4.875	1175	1177	1181	rVB	124	70	0.00%	0.000%
8	4.897	1181	1184	1186	rBV	91	56	0.00%	0.000%
9	5.007	1216	1218	1221	rVB	75	41	0.00%	0.000%
10	5.100	1229	1247	1268	rBV2	224820	539449	1.09%	0.999%
11	5.428	1348	1349	1351	rVB2	185	62	0.00%	0.000%
12	5.444	1351	1354	1356	rBV	139	47	0.00%	0.000%
13	5.486	1364	1367	1372	rVB	126	110	0.00%	0.000%
14	5.524	1377	1379	1380	rBV	145	60	0.00%	0.000%
15	5.569	1388	1393	1398	rBV	64	87	0.00%	0.000%
16	5.669	1409	1424	1447	rBV	208376	408779	0.83%	0.757%
17	5.955	1505	1513	1520	rBV3	995	1489	0.00%	0.003%
18	5.984	1520	1522	1524	rVB3	143	53	0.00%	0.000%
19	5.997	1524	1526	1530	rBV	79	47	0.00%	0.000%
20	6.125	1552	1566	1594	rBV	119144	243412	0.49%	0.451%
21	6.492	1677	1680	1691	rVB	100	109	0.00%	0.000%
22	6.611	1714	1717	1719	rBV	51	38	0.00%	0.000%
23	6.624	1719	1721	1724	rVB	203	108	0.00%	0.000%
24	6.637	1724	1725	1726	rBV	105	37	0.00%	0.000%
25	6.656	1727	1731	1736	rVB2	256	263	0.00%	0.000%
26	6.717	1747	1750	1752	rBV	55	34	0.00%	0.000%
27	6.752	1756	1761	1764	rBV	68	67	0.00%	0.000%
28	6.849	1788	1791	1795	rBV	57	51	0.00%	0.000%
29	6.907	1807	1809	1812	rVB	93	55	0.00%	0.000%
30	6.929	1812	1816	1821	rBV	118	151	0.00%	0.000%
31	7.035	1836	1849	1876	rBV	61739	109152	0.22%	0.202%
32	7.158	1883	1887	1888	rBV	181	119	0.00%	0.000%
33	7.174	1889	1892	1893	rVV3	528	325	0.00%	0.001%
34	7.190	1893	1897	1906	rVB3	1531	2220	0.00%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092318\
 Data File : VV007764.D
 Acq On : 23 Sep 2018 04:15
 Operator : SY/MD
 Sample : J5013-04
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C08T2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092318WMA.M
 Title : VOC Analysis

35	7.312	1932	1935	1937	rVB2	137	75	0.00%	0.000%
36	7.363	1937	1951	1980	rBV	270504	478072	0.97%	0.886%
37	7.547	2006	2008	2009	rBV	172	71	0.00%	0.000%
38	7.669	2035	2046	2063	rBV	43668	72346	0.15%	0.134%
39	7.781	2079	2081	2085	rVB	193	100	0.00%	0.000%
40	7.839	2095	2099	2102	rBV2	175	182	0.00%	0.000%
41	8.084	2172	2175	2178	rBV	118	65	0.00%	0.000%
42	8.138	2181	2192	2228	rBV2	122855	242274	0.49%	0.449%
43	8.479	2296	2298	2300	rBV	117	68	0.00%	0.000%
44	8.611	2338	2339	2341	rVB	119	44	0.00%	0.000%
45	8.669	2353	2357	2359	rBV	87	69	0.00%	0.000%
46	8.682	2359	2361	2366	rVV	225	146	0.00%	0.000%
47	8.788	2389	2394	2397	rVB	77	65	0.00%	0.000%
48	8.807	2397	2400	2404	rBV	165	77	0.00%	0.000%
49	8.833	2404	2408	2414	rBV	109	136	0.00%	0.000%
50	8.900	2416	2429	2459	rBV	311982	522637	1.06%	0.968%
51	9.096	2487	2490	2493	rBV3	216	159	0.00%	0.000%
52	9.161	2507	2510	2513	rBV	170	99	0.00%	0.000%
53	9.186	2513	2518	2525	rVB	401	528	0.00%	0.001%
54	9.267	2541	2543	2544	rBV	98	41	0.00%	0.000%
55	9.309	2552	2556	2560	rBV	87	81	0.00%	0.000%
56	9.395	2580	2583	2589	rBV	52	70	0.00%	0.000%
57	9.588	2640	2643	2647	rBV2	256	197	0.00%	0.000%
58	9.701	2675	2678	2681	rBV	72	51	0.00%	0.000%
59	9.820	2712	2715	2716	rBV	57	34	0.00%	0.000%
60	9.855	2723	2726	2729	rBV	126	92	0.00%	0.000%
61	9.875	2730	2732	2734	rVB	163	67	0.00%	0.000%
62	9.984	2759	2766	2770	rBV2	278	380	0.00%	0.001%
63	10.045	2779	2785	2787	rBV	114	100	0.00%	0.000%
64	10.193	2828	2831	2833	rBV	95	67	0.00%	0.000%
65	10.267	2841	2854	2872	rBV	181098	290038	0.59%	0.537%
66	10.421	2897	2902	2904	rBV2	319	335	0.00%	0.001%
67	10.608	2958	2960	2962	rVB	139	43	0.00%	0.000%
68	10.669	2977	2979	2983	rBV	83	54	0.00%	0.000%
69	10.807	3020	3022	3025	rVB	185	68	0.00%	0.000%
70	10.823	3025	3027	3028	rBV	110	60	0.00%	0.000%
71	10.875	3041	3043	3046	rVB	155	64	0.00%	0.000%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092318\
 Data File : VV007764.D
 Acq On : 23 Sep 2018 04:15
 Operator : SY/MD
 Sample : J5013-04
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C08T2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092318WMA.M
 Title : VOC Analysis

72	10.952	3061	3067	3069	rBV	87	86	0.00%	0.000%
73	10.971	3070	3073	3074	rBV	255	114	0.00%	0.000%
74	11.064	3099	3102	3107	rBV	134	106	0.00%	0.000%
75	11.231	3143	3154	3163	rBV5	2524	3884	0.01%	0.007%
76	11.299	3163	3175	3204	rVV	331977	558244	1.13%	1.034%
77	11.463	3224	3226	3228	rVB	140	58	0.00%	0.000%
78	11.592	3257	3266	3274	rBV5	1123	1893	0.00%	0.004%
79	11.675	3280	3292	3314	rBV	297810	518130	1.05%	0.960%
80	11.772	3318	3322	3324	rBV	189	84	0.00%	0.000%
81	11.788	3324	3327	3329	rVB	128	70	0.00%	0.000%
82	11.804	3329	3332	3336	rBV	171	120	0.00%	0.000%
83	11.881	3351	3356	3361	rVB2	160	149	0.00%	0.000%
84	11.926	3366	3370	3374	rBV2	140	146	0.00%	0.000%
85	11.993	3387	3391	3394	rBB2	160	106	0.00%	0.000%
86	12.010	3394	3396	3398	rVB	158	45	0.00%	0.000%
87	12.026	3399	3401	3404	rBV2	160	115	0.00%	0.000%
88	12.145	3435	3438	3442	rVB	214	155	0.00%	0.000%
89	12.315	3489	3491	3493	rBV	154	91	0.00%	0.000%
90	12.360	3501	3505	3506	rBV	218	129	0.00%	0.000%
91	12.399	3514	3517	3521	rVB	295	111	0.00%	0.000%
92	12.550	3560	3564	3567	rBV2	197	139	0.00%	0.000%
93	12.563	3567	3568	3571	rBV	136	81	0.00%	0.000%
94	12.698	3602	3610	3612	rBV4	890	910	0.00%	0.002%
95	12.768	3626	3632	3637	rBV2	235	299	0.00%	0.001%
96	12.903	3672	3674	3676	rBV	164	115	0.00%	0.000%
97	13.013	3705	3708	3710	rBV	194	137	0.00%	0.000%
98	13.318	3795	3803	3813	rBB3	4364	6557	0.01%	0.012%
99	13.466	3845	3849	3851	rBV	304	191	0.00%	0.000%
100	13.804	3947	3954	3962	rBV4	1902	2403	0.00%	0.004%


Sum of corrected areas: 53974972

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV092318\
Data File : VV007764.D
Acq On : 23 Sep 2018 04:15
Operator : SY/MD
Sample : J5013-04
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C08T2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092318WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

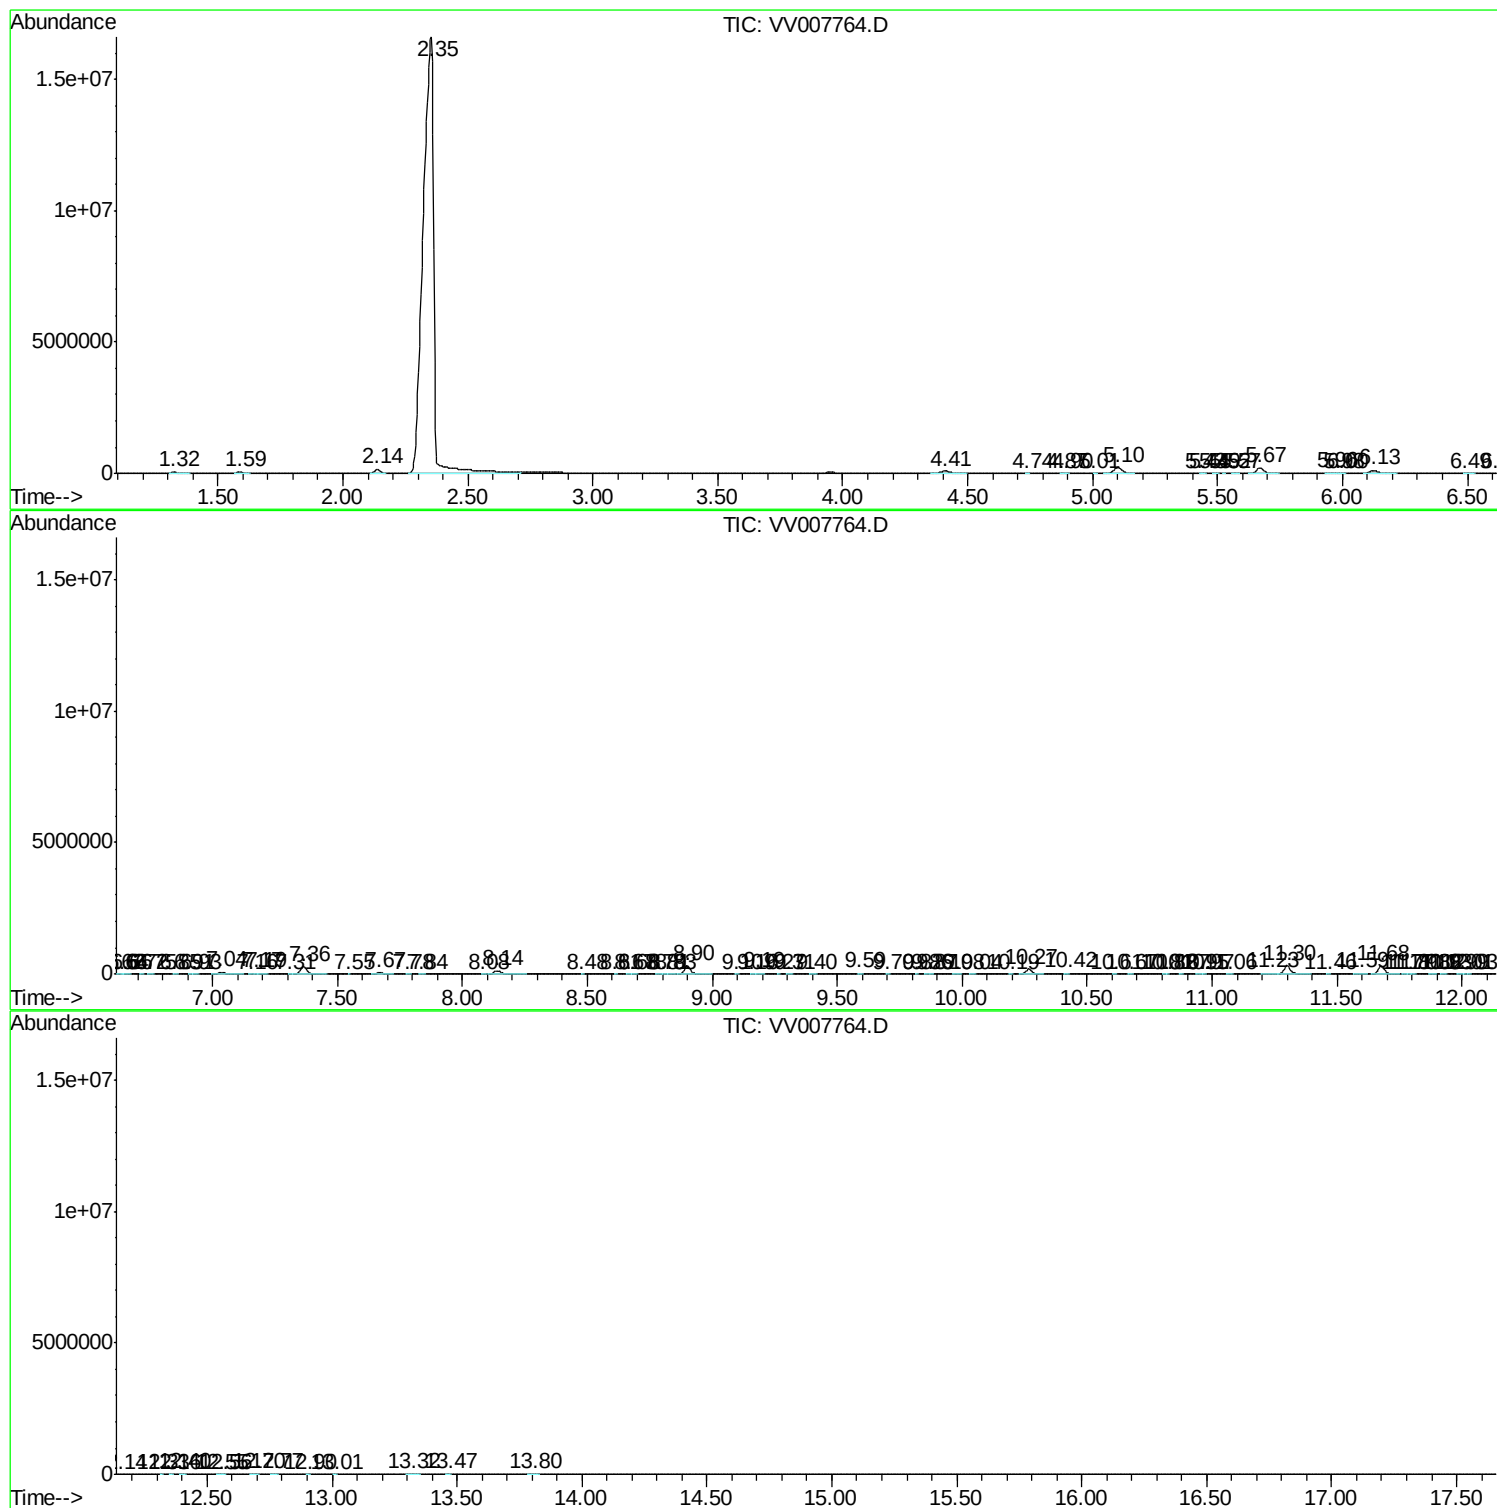

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV092318\
Data File : VV007764.D
Acq On : 23 Sep 2018 04:15
Operator : SY/MD
Sample : J5013-04
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C08T2










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092318WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.35	6041.54 ug/L	49393100	1,4-Difluorobenzene	5.67

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Isopropyl Alcohol	60	C3H8O	000067-63-0	78
2		Isopropyl Alcohol	60	C3H8O	000067-63-0	78
3		Isopropyl Alcohol	60	C3H8O	000067-63-0	78
4		Isopropyl Alcohol	60	C3H8O	000067-63-0	9
5		Hydrazine, 1,2-dimethyl-	60	C2H8N2	000540-73-8	9

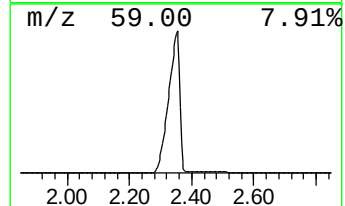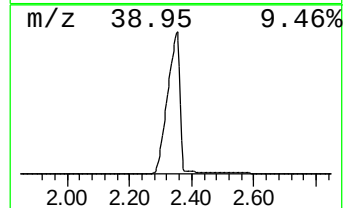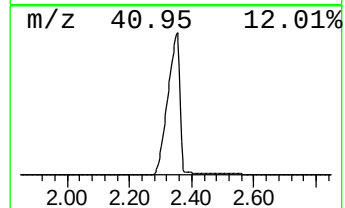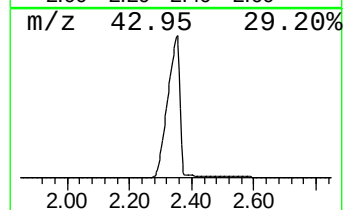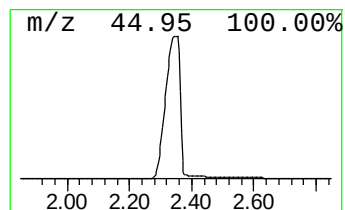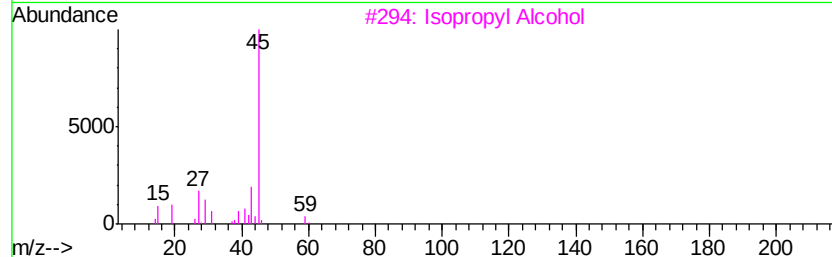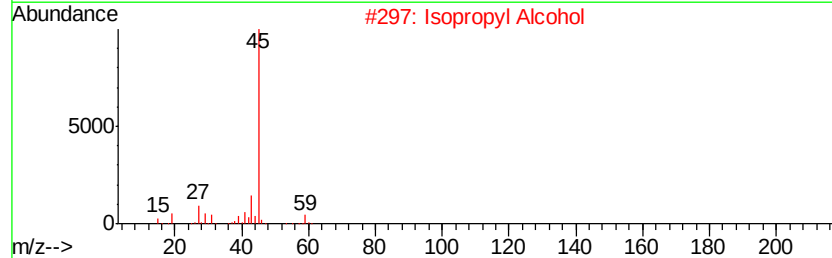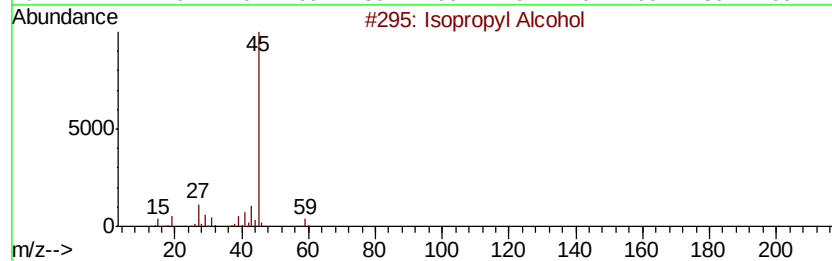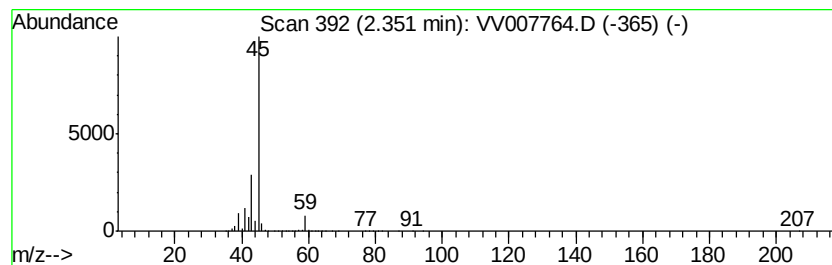

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV092318\
Data File : VV007764.D
Acq On : 23 Sep 2018 04:15
Operator : SY/MD
Sample : J5013-04
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C08T2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092318WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.35	6041.5	ug/L	49393100	1	5.67	408779	50.0