

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092318\
 Data File : VV007766.D
 Acq On : 23 Sep 2018 05:05
 Operator : SY/MD
 Sample : J5013-06
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C08T8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092318WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.322	64	72	90	rVB	75618	78223	13.21%	1.592%
2	1.586	147	154	168	rVB	73142	84912	14.34%	1.728%
3	2.135	315	325	337	rBV	174847	252257	42.59%	5.133%
4	2.306	370	378	396	rVB	37696	62022	10.47%	1.262%
5	3.389	713	715	719	rBV	214	115	0.02%	0.002%
6	3.949	875	889	915	rBV	38213	104680	17.67%	2.130%
7	4.319	1002	1004	1007	rBV2	152	117	0.02%	0.002%
8	4.409	1014	1032	1060	rBV	94811	236464	39.92%	4.812%
9	4.653	1105	1108	1112	rVB	208	121	0.02%	0.002%
10	4.679	1112	1116	1125	rVB	117	134	0.02%	0.003%
11	4.721	1125	1129	1132	rBV	114	121	0.02%	0.002%
12	4.859	1169	1172	1179	rBV	1905	1138	0.19%	0.023%
13	4.917	1186	1190	1194	rVB	135	119	0.02%	0.002%
14	5.103	1230	1248	1281	rBV2	239091	592303	100.00%	12.052%
15	5.421	1345	1347	1351	rBV2	153	142	0.02%	0.003%
16	5.528	1377	1380	1383	rVB	186	107	0.02%	0.002%
17	5.595	1391	1401	1405	rBV2	250	383	0.06%	0.008%
18	5.672	1405	1425	1457	rBV	196910	395562	66.78%	8.049%
19	5.817	1468	1470	1479	rVB3	287	325	0.05%	0.007%
20	5.949	1503	1511	1512	rBV3	1159	1161	0.20%	0.024%
21	6.126	1552	1566	1586	rBV	128616	260764	44.03%	5.306%
22	6.483	1673	1677	1681	rBV	115	104	0.02%	0.002%
23	6.627	1720	1722	1725	rVV	279	205	0.03%	0.004%
24	6.647	1725	1728	1739	rVB4	534	732	0.12%	0.015%
25	6.714	1746	1749	1754	rVB	150	131	0.02%	0.003%
26	6.753	1754	1761	1766	rVB	71	105	0.02%	0.002%
27	6.788	1766	1772	1774	rBV	186	128	0.02%	0.003%
28	6.859	1791	1794	1798	rVV	175	124	0.02%	0.003%
29	6.888	1798	1803	1811	rVB	81	101	0.02%	0.002%
30	7.036	1837	1849	1869	rBV	64676	115615	19.52%	2.353%
31	7.135	1878	1880	1884	rVB2	373	262	0.04%	0.005%
32	7.193	1884	1898	1908	rVB7	1798	3144	0.53%	0.064%
33	7.364	1938	1951	1980	rBV	288137	517391	87.35%	10.528%
34	7.598	2021	2024	2025	rBV	235	130	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092318\
 Data File : VV007766.D
 Acq On : 23 Sep 2018 05:05
 Operator : SY/MD
 Sample : J5013-06
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C08T8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092318WMA.M
 Title : VOC Analysis

35	7.669	2034	2046	2070	rVV	45765	78611	13.27%	1.600%
36	7.804	2085	2088	2092	rBV	167	123	0.02%	0.003%
37	7.881	2107	2112	2116	rVV2	175	197	0.03%	0.004%
38	7.981	2138	2143	2144	rBV	251	212	0.04%	0.004%
39	8.138	2180	2192	2231	rBV	119020	254972	43.05%	5.188%
40	8.473	2292	2296	2299	rBV	123	100	0.02%	0.002%
41	8.502	2302	2305	2310	rVV2	224	172	0.03%	0.003%
42	8.544	2313	2318	2320	rVB	182	136	0.02%	0.003%
43	8.900	2417	2429	2467	rBV	294286	499325	84.30%	10.160%
44	9.106	2490	2493	2501	rVB4	673	765	0.13%	0.016%
45	9.187	2512	2518	2524	rVB2	202	215	0.04%	0.004%
46	9.489	2609	2612	2614	rBV	170	103	0.02%	0.002%
47	9.505	2614	2617	2621	rBV	171	115	0.02%	0.002%
48	9.585	2637	2642	2644	rBV	186	130	0.02%	0.003%
49	9.637	2654	2658	2663	rBV	111	117	0.02%	0.002%
50	10.010	2772	2774	2781	rVB	192	105	0.02%	0.002%
51	10.090	2793	2799	2801	rBV	144	152	0.03%	0.003%
52	10.216	2831	2838	2841	rBV	173	122	0.02%	0.002%
53	10.267	2841	2854	2883	rVV	190457	311855	52.65%	6.346%
54	10.425	2900	2903	2905	rBV	206	151	0.03%	0.003%
55	10.515	2924	2931	2934	rVB	215	136	0.02%	0.003%
56	10.540	2934	2939	2941	rBV2	168	114	0.02%	0.002%
57	10.769	3007	3010	3017	rVB	114	113	0.02%	0.002%
58	10.852	3033	3036	3041	rVB	104	102	0.02%	0.002%
59	10.942	3062	3064	3066	rBV	164	113	0.02%	0.002%
60	10.981	3071	3076	3077	rBV2	322	284	0.05%	0.006%
61	11.174	3133	3136	3144	rVB	117	120	0.02%	0.002%
62	11.232	3150	3154	3160	rVB2	655	667	0.11%	0.014%
63	11.299	3160	3175	3201	rBV	307529	516470	87.20%	10.509%
64	11.560	3250	3256	3260	rBV	126	138	0.02%	0.003%
65	11.598	3260	3268	3275	rVB3	842	1178	0.20%	0.024%
66	11.678	3275	3293	3317	rBV	306319	530047	89.49%	10.785%
67	11.804	3330	3332	3335	rVV	214	130	0.02%	0.003%
68	11.823	3335	3338	3345	rVV	88	108	0.02%	0.002%
69	11.894	3353	3360	3363	rBV	193	235	0.04%	0.005%
70	11.997	3388	3392	3396	rBV2	167	150	0.03%	0.003%
71	12.093	3421	3422	3425	rBV2	284	106	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092318\
 Data File : VV007766.D
 Acq On : 23 Sep 2018 05:05
 Operator : SY/MD
 Sample : J5013-06
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C08T8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092318WMA.M
 Title : VOC Analysis

72	12.125	3429	3432	3433	rBV	182	106	0.02%	0.002%
73	12.232	3460	3465	3467	rBV	237	216	0.04%	0.004%
74	12.283	3477	3481	3487	rVB2	261	205	0.03%	0.004%
75	12.328	3487	3495	3498	rBV2	257	358	0.06%	0.007%
76	12.492	3542	3546	3550	rVV	252	230	0.04%	0.005%
77	12.514	3550	3553	3558	rVB	249	221	0.04%	0.004%
78	12.563	3562	3568	3570	rBV2	256	220	0.04%	0.004%
79	12.601	3578	3580	3582	rBV	150	106	0.02%	0.002%
80	12.627	3586	3588	3593	rVB	258	180	0.03%	0.004%
81	12.653	3593	3596	3600	rBV2	202	211	0.04%	0.004%
82	12.701	3608	3611	3622	rVB4	577	682	0.12%	0.014%
83	12.759	3622	3629	3632	rBV2	182	233	0.04%	0.005%
84	12.778	3632	3635	3639	rBV	163	116	0.02%	0.002%
85	12.804	3639	3643	3645	rBV2	194	162	0.03%	0.003%
86	12.894	3669	3671	3674	rBV2	154	107	0.02%	0.002%
87	12.913	3674	3677	3680	rVB	166	111	0.02%	0.002%
88	12.936	3680	3684	3689	rBV	183	199	0.03%	0.004%
89	13.048	3715	3719	3721	rBV2	265	245	0.04%	0.005%
90	13.084	3726	3730	3733	rBV	194	187	0.03%	0.004%
91	13.322	3797	3804	3810	rVB3	777	1025	0.17%	0.021%
92	13.408	3827	3831	3833	rBV	155	144	0.02%	0.003%
93	13.543	3871	3873	3876	rBV	159	102	0.02%	0.002%
94	13.566	3876	3880	3885	rVB2	244	282	0.05%	0.006%
95	13.768	3940	3943	3945	rBV2	172	124	0.02%	0.003%
96	13.807	3950	3955	3961	rBV3	496	521	0.09%	0.011%
97	14.006	4011	4017	4020	rBV2	289	323	0.05%	0.007%
98	14.151	4059	4062	4069	rBV2	213	271	0.05%	0.006%
99	14.701	4231	4233	4237	rVB2	419	230	0.04%	0.005%
100	14.907	4295	4297	4302	rBV	255	174	0.03%	0.004%


Sum of corrected areas: 4914522

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV092318\
Data File : VV007766.D
Acq On : 23 Sep 2018 05:05
Operator : SY/MD
Sample : J5013-06
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C08T8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092318WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

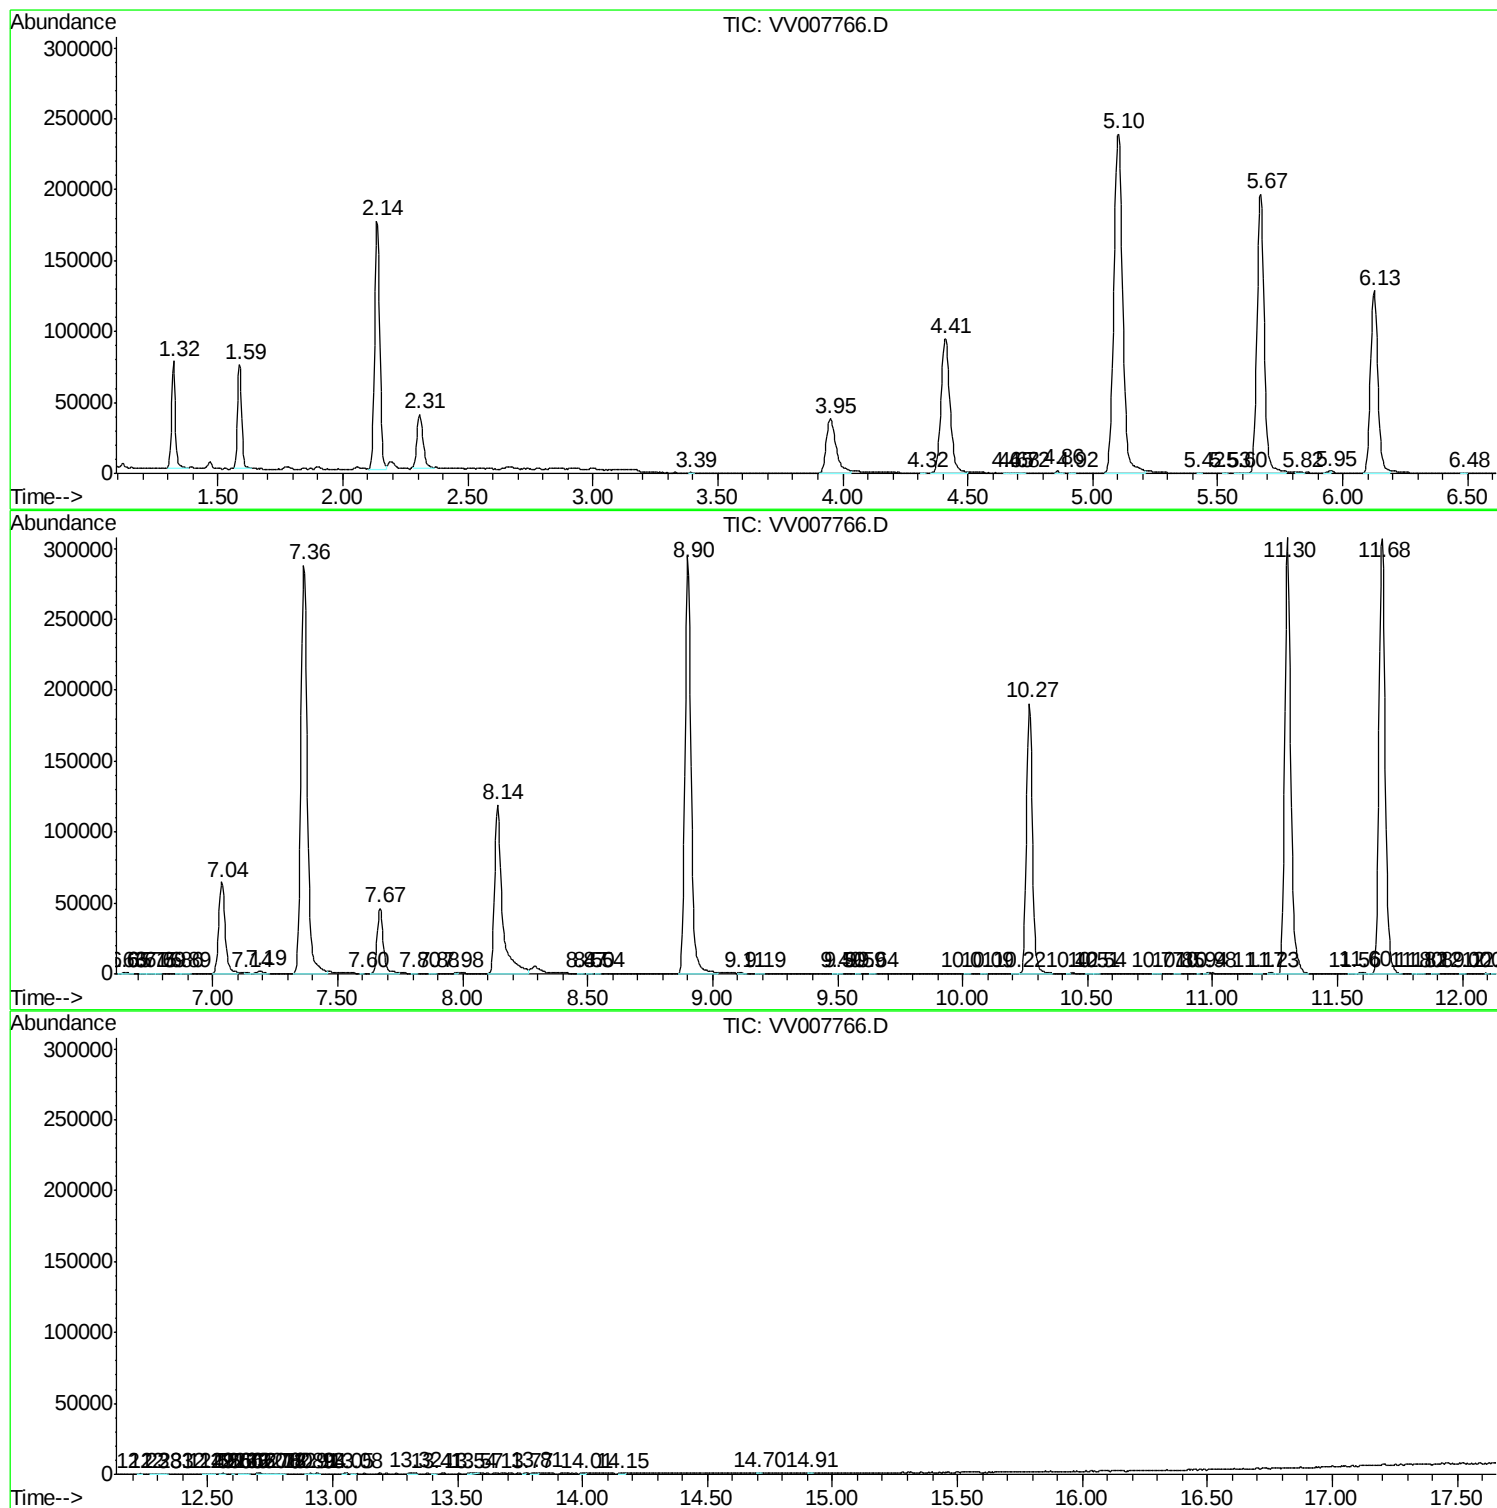

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV092318\
Data File : VV007766.D
Acq On : 23 Sep 2018 05:05
Operator : SY/MD
Sample : J5013-06
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C08T8










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092318WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.31	7.84 ug/L	62022	1,4-Difluorobenzene	5.67

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	78
2			Isopropyl Alcohol	60	C3H8O	000067-63-0	78
3			Isopropyl Alcohol	60	C3H8O	000067-63-0	72
4			Isopropyl Alcohol	60	C3H8O	000067-63-0	72
5			Hydrazine, 1,2-dimethyl-	60	C2H8N2	000540-73-8	9

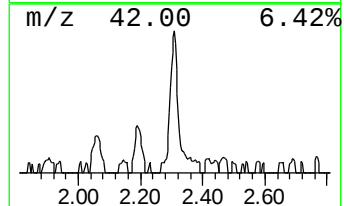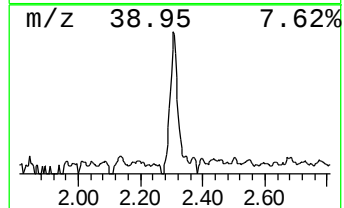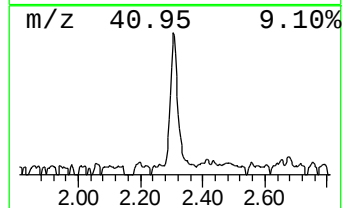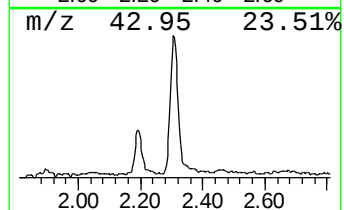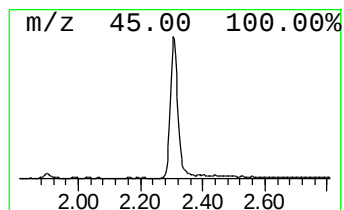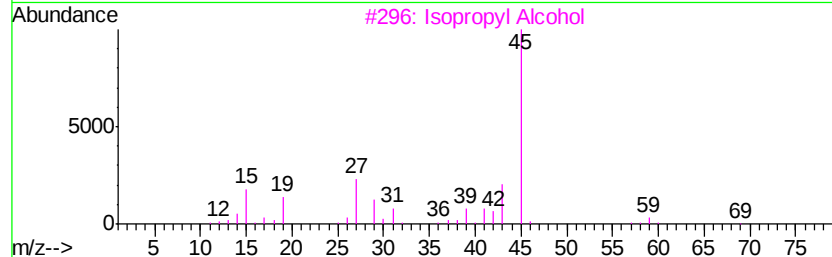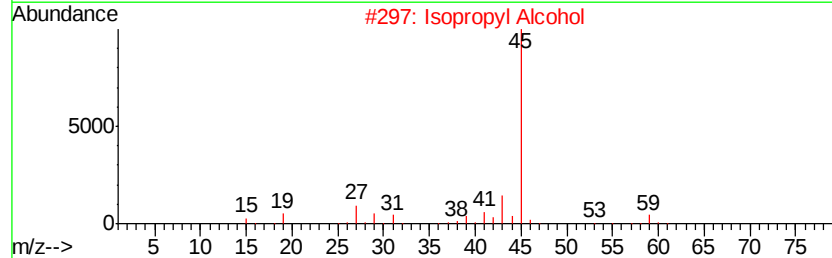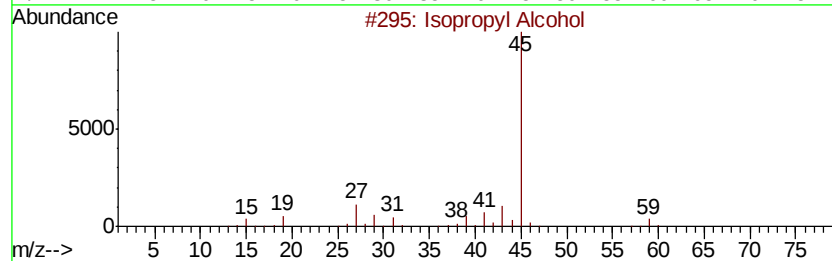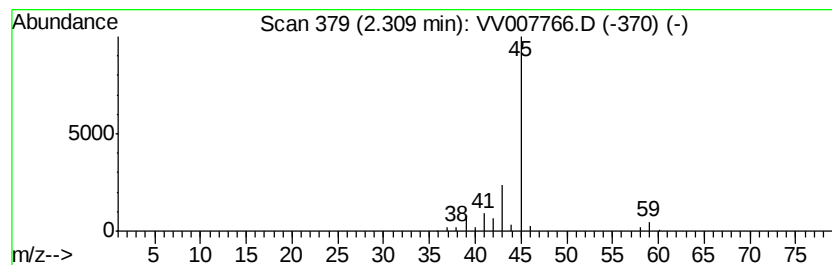

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV092318\
Data File : VV007766.D
Acq On : 23 Sep 2018 05:05
Operator : SY/MD
Sample : J5013-06
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C08T8

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092318WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.31	7.8	ug/L	62022	1	5.67	395562	50.0